

Life moves us



SURGICAL TECHNIQUE



REVERE® ADDITION®

Revision System

GLOBUS MEDICAL

Outside the US Only



Life moves us

At Globus, we move with a sense of urgency to deliver innovations that improve the quality of life for patients with spinal disorders. We are inspired by the needs of these patients and also the needs of the surgeons and health care providers who treat them.

This passion combined with Globus' world class engineering transforms clinical insights into tangible spine care solutions. We are driven to provide the highest quality products to improve the techniques and outcomes of spine surgery so patients can resume their lives as quickly as possible. We extend our reach beyond our world class implants, instrumentation, and service by partnering with researchers and educators to advance the science and knowledge of spine care.

The energy and enthusiasm each of us bring everyday to Globus is palpable. We are constantly in the pursuit of better patient care and understand that speed is critical because life cannot wait.

GLOBUS
MEDICAL

www.globusmedical.com

REVERE® ADDITION®

Revision System







REVERE® ADDITION® is a thoracolumbar revision system that is designed to reduce the trauma associated with revision surgeries by eliminating the need to remove existing implants.

REVERE® ADDITION® includes a wide variety of rod-to-rod connectors to form a rigid connection. The system features unique REVERE® RESCUE® implants to securely attach to existing REVERE®, CREO®, BEACON®, and PROTEX® 5.5mm through 6.5mm rod constructs to help reduce anatomic disruption, while saving significant implant costs.

REVERE® ADDITION® Revision System
DISTINGUISHING CHARACTERISTICS

Comprehensive Implant Options


REVERE® RESCUE® Clamps

- Unique implants designed to attach to existing 5.5mm through 6.5mm rod constructs with an integrated rod for extension
- Includes In-Line, Offset, and U Extension Clamps



Rod-to-Rod Connectors

- Connection options for smaller one to two-level constructs
- Includes open-ended, closed-ended, and Y connectors in multiple sizes

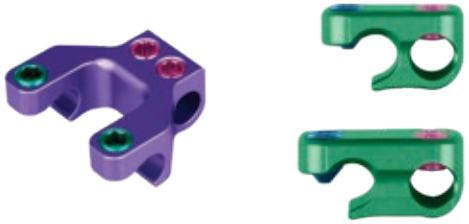

Innovative Design

This system is designed for construct compatibility with existing 5.5mm through 6.5mm REVERE®, CREO®, BEACON®, or PROTEX® implants.

The clamps may be used for in-line and offset connections for revision surgery, medial or lateral.



REVERE® 6.35 and REVERE® ADDITION®



BEACON® ML and REVERE® ADDITION®



PROTEX® and REVERE® ADDITION®

CONTENTS

Implant Overview 4

Examples of Revision Constructs 6

Instrument Overview 8

Surgical Technique

- 1. Preoperative Planning 13
- 2. Approach 13
- 3. Implant Selection 13
- 4. Implant Trialing 14
- 5. Implant Insertion 16
  - *REVERE® RESCUE® Clamp Insertion* 16
  - *Using the REVERE® RESCUE® Bender* 18
  - *Rod-to-Rod Connector Insertion* 20
- 6. Compression or Distraction 22
- 7. Final Tightening 23

Final Constructs 23

REVERE® ADDITION® Revision System Connectors Guide 24

REVERE® ADDITION® Revision System Set 26

REVERE® ADDITION® Revision System Stainless Steel Set 30



The Surgical Technique shown is for illustrative purposes only. The technique(s) actually employed in each case always depends on the medical judgment of the surgeon exercised before and during surgery as to the best mode of treatment for each patient. Additionally, as instruments may occasionally be updated, the instruments depicted in this Surgical Technique may not be exactly the same as the instruments currently available. Please consult with your sales representative or contact Globus directly for more information.

IMPLANT OVERVIEW

REVERE® RESCUE® CLAMPS

In-Line Extension Clamp



- Provides direct in-line connection
- Integrated 200mm rod
- Mechanically stronger critical junction where the rod meets the clamp
- Available in titanium alloy and stainless steel

Offset Extension Clamp



- Provides 7.5mm offset connection
- Integrated 200mm rod
- Available in titanium alloy and stainless steel

U-Connector



- Shorter run-on-rod on each side of the set screw
- Offsets medially or laterally depending on anatomical requirements
- Integrated 200mm rod
- Accommodate lordosis of the existing rod
- 6.35mm U-Connector is pre-curved to minimize *in situ* bending
- Available in titanium alloy and stainless steel

COLOR CODING

	Violet: connects to 5.5–6.0mm rods; 5.5mm rod extending from implant
	Fuchsia: connects to 6.0–6.5mm rods; 5.5mm rod extending from implant
	Green: connects to 6.0–6.35mm rods; 6.35mm rod extending from implant

IMPLANT OVERVIEW

ROD-TO-ROD CONNECTORS

In-Line Connectors

- Allow for two rods to be joined end-to-end
- May be used with REVERE® RESCUE® Clamps or additional 5.5–6.5mm rod constructs to enhance stability
- Available in titanium alloy and stainless steel



Parallel Connectors

- Closed connector for 5.5–6.5mm rods
- Available in standard, wide, extra wide sizes
- Single and double set screw configurations
- Available in titanium alloy and stainless steel



Rod-to-Rod Clamps

- Open clamps for 5.5–6.5mm rods
- Open end is assembled over existing and new rods
- Available in single or double set screw formats with various offset widths
- Configurations to secure both 5.5mm and 6.35mm rods in the same clamp
- Available in titanium alloy and stainless steel



Parallel Connector Clamps

- Open clamp on one end and closed connector on the other
- Open end is assembled over the existing rod; new rod slides through closed end
- Available as Y Offset Connectors and single or double set screw styles with various offset widths
- Configurations to secure both 5.5mm and 6.35mm rods in the same clamp
- Available in titanium alloy and stainless steel



EXAMPLES OF REVISION CONSTRUCTS


In-Line Extension Clamp






U-Connectors



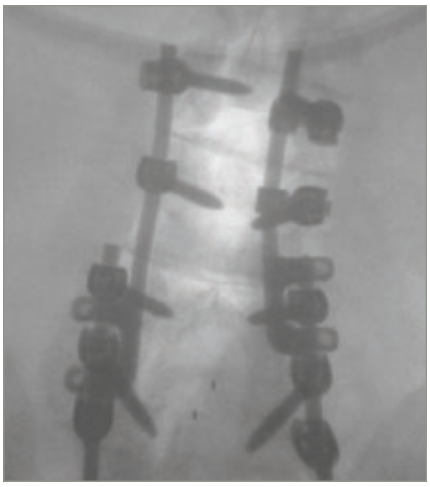


Rod-to-Rod Connectors



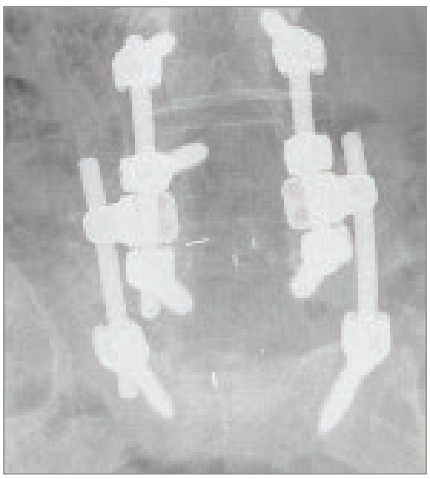

Y Offset Connector



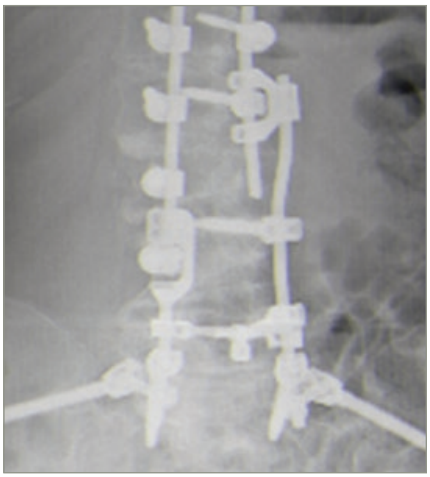

Offset Extension Clamps



INSTRUMENT OVERVIEW

Trials




Trial, U-Connector 654.405




Trial, In-Line Connector, Left 654.406



Trial, In-Line Connector, Right 654.407

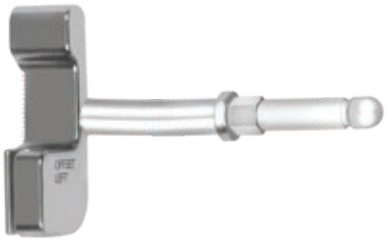

Trial, Offset Connector, Left 654.408

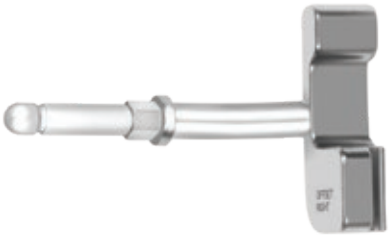

Trial, Offset Connector, Right 654.409



Trial, Quick Connect Handle 654.411

Trials (cont'd)



Trial, 15mm Screw Gap 654.404



Rod Template, 150mm 602.501

Set Screw Tightening Instruments



3.5mm Torque Limiting Hex Driver 654.415



3.5mm Hex Driver, Self-Retaining 624.406*

**Additionally available in REVERE® Stabilization System*

Rod Manipulation Instruments



REVERE® RESCUE® Bender 654.410



Rod Bender, Left 652.690



Rod Bender, Right 652.691



Rod Holder 624.510*



Rod Gripper 602.522**


**Additionally available in REVERE® Stabilization System*
***Additionally available in PROTEX® Stabilization System*

Rod Manipulation Instruments (Cont'd)



Rod Cutter 602.508**

Compression/Distraction Instruments

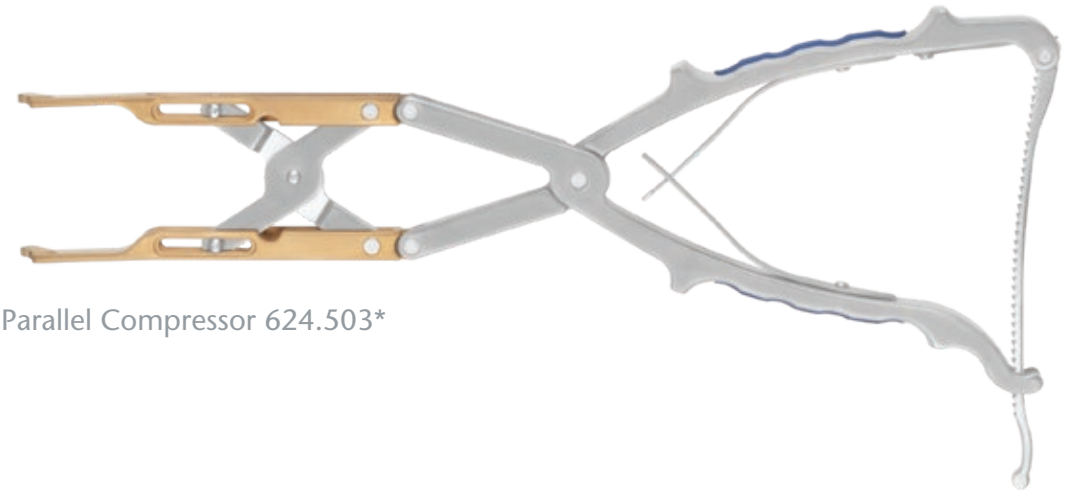

Parallel Compressor 624.503*



Parallel Distractor 624.504*

**Additionally available in REVERE® Stabilization System*
***Additionally available in PROTEX® Stabilization System*

Recommended sets to be used with REVERE® ADDITION® Revision System

For All Cases

- REVERE® ADDITION® Revision Fixation System (954.910 or 954.920)
- Universal Implant Removal Set (954.901)

REVERE® 5.5mm

- REVERE® Implants (924.901 or 924.931)
- REVERE® Instruments I (924.902)
- REVERE® Instruments II (924.903)
- REVERE® Dual Outer Diameter Polyaxial Screw Set (924.923)
- 5.5mm: *In Situ* Benders—Coronal (624.309/624.310) and Sagittal (624.303/624.304)

REVERE® 6.35mm

- REVERE® 6.35 Implants (934.901)
- REVERE® 6.35 Instruments I (934.902)
- REVERE® 6.35 Instruments II (934.903)
- REVERE® 6.35 Dual Outer Diameter Polyaxial Screw Set (934.923)
- 6.35mm: *In Situ* Benders – Coronal (634.309/634.310) and Sagittal (634.303/634.304)

Also Recommended

- REVERE® Deformity Instruments (924.904)
- REVERE® Deformity Implants, Monoaxial Screws (924.905)
- REVERE® 6.35 Deformity Instruments (934.904)
- REVERE® 6.35 Deformity Implants, Monoaxial Screws (934.905)
- Table-top Rod Cutter (602.508)
- *In Situ* Rod Cutter, and Vise Grips
- REVERE® ADDITION® Sacroiliac Fixation System (954.911)

Stainless Steel

- SS REVERE® ADDITION® Revision Fixation System (954.912)
- SS REVERE® Implant Set (924.909) with 3.5mm Hex Driver, Torque Limiting, SS (624.611)
- SS REVERE® 6.35 Implant Set (934.909) with 3.5mm Torque Limiting Driver, SS (634.611)
- SS REVERE® 6.35 Dual Outer Diameter Polyaxial Screw Set (934.924)
- SS REVERE® ADDITION® Sacroiliac Fixation System (954.913)

REVERE® ADDITION® REVISION SYSTEM
SURGICAL TECHNIQUE

Step 1 Preoperative Planning

Preview the existing construct to determine which REVERE®, CREO®, BEACON®, or PROTEX® implants are present using X-ray AP and lateral radiographs for surgical planning. Determine the desired revision method and implants.

Step 2 Approach

The patient is placed under anesthesia and positioned prone. The operative area is carefully cleaned, and an incision is made to expose the last one or two levels, distal, with existing hardware. Lateral C-arm fluoroscopy or other radiographic methods may be used throughout surgery to ensure correct implant placement.

Please refer to the specific product insert for additional information.

Pedicle screws are inserted into the exposed level(s) for the revision procedure. For pedicle screw insertion, refer to the REVERE® Stabilization System Surgical Technique (GMTGD17OU).

Step 3 Implant Selection

REVERE® RESCUE® Clamps and Rod-to-Rod Connectors are two available options for hardware connection. Consider the following when selecting implants:

REVERE® RESCUE® Clamps

- Number of additional levels to be addressed
- Rod spacing available to accommodate the clamp
- Amount of lateral offset, if required
- Surgeon preference



Rod-to-Rod Connectors

- May be a part of any revision plan
- Specific construct geometry needed (e.g. parallel support)
- May be used in conjunction with other revision implants, such as REVERE® RESCUE® Clamps or pelvic fixation for multiple connection points




Step 4 Implant Trialing

Trialing is an optional step in the procedure to determine the appropriate head configuration and the available spacing for the clamps and connectors prior to implantation. Attach the **Trial, Quick Connect Handle** to the desired trial. Refer to the table on page 15 for minimum spacing requirements.


Assembling the Implant Trial

Grasp the Trial, Quick Connect Handle and pull back the ridged grip of the retaining sleeve. Hold the trial attachment in the other hand and insert it into the handle. Rotate the trial until the hexagonal end is fully engaged and release the retaining sleeve. The trial is now securely locked into the handle.

For removal, pull back the retaining sleeve with one hand to release the trial and gently pull out the trial with the other hand.

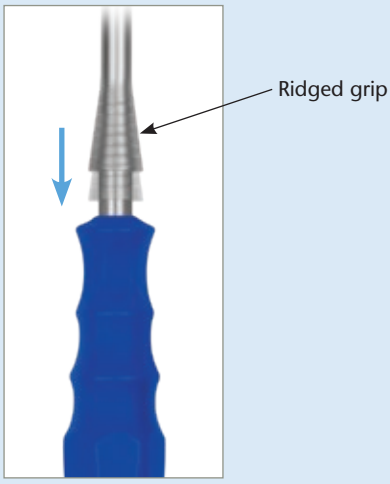

Pulling back the retaining sleeve

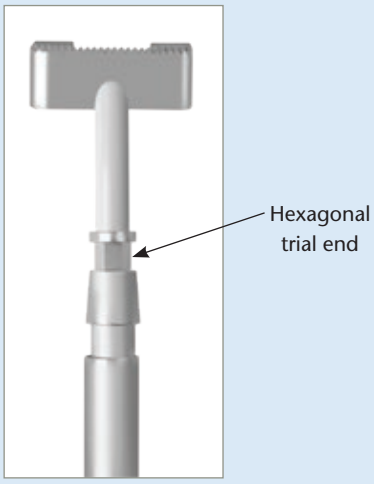

Hexagonal end attached to the handle






Trial fully engaged in handle

The **Trial, 15mm Screw Gap** is designed with an attached handle and may also be used to measure the rod space between screws.




Trial, 15mm Screw Gap

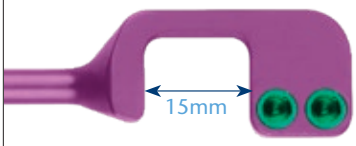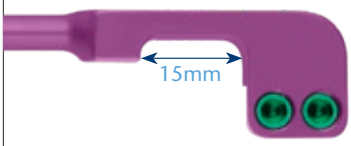Criteria for REVERE® Rescue Clamps		
Type	**Space Between Exposed Screws**	**Note**
In-Line Extension Clamp 	≥15mm	Requires 5mm or less of rod extending from the last screw head
Offset Extension Clamp 	≥15mm	Provides approximately 7.5mm of lateral offset
U-Connector 	≥8mm	Designed to accommodate lordosed and curved rods

A larger clamp size may be needed for highly lordotic lower lumbar constructs to accommodate rod curvature, particularly with in-line and offset REVERE® RESCUE® Clamps.

Align the screw head opening on the selected trial with the exposed screw head on the existing construct. Position the trial such that the existing rod is seated in the trial's rod opening. Select the corresponding implant based on the size and style of the trial.

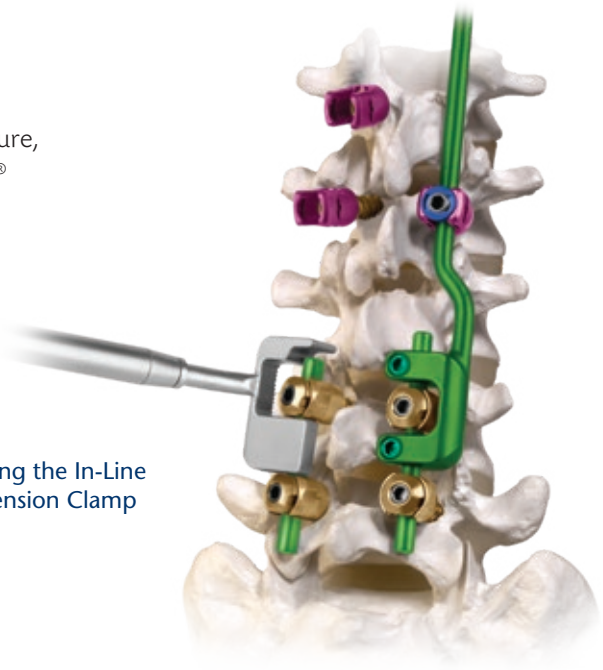


Trialing the In-Line Extension Clamp

Step 5 Implant Insertion

REVERE® RESCUE® Clamp Insertion

Examine the pedicle screw placement to determine the necessary rod length and contour. Using the **REVERE® RESCUE® Bender**, contour the extending rod of the REVERE® RESCUE® Clamp (medial lateral, lordotic, or kyphotic) based on patient anatomy. Using the **Table Top Rod Cutter,** provisionally cut the rod to length. Leave a minimum of 50mm of rod for bending.

Note: Refer to page 18–19 for additional usage information on the REVERE® RESCUE® Bender.

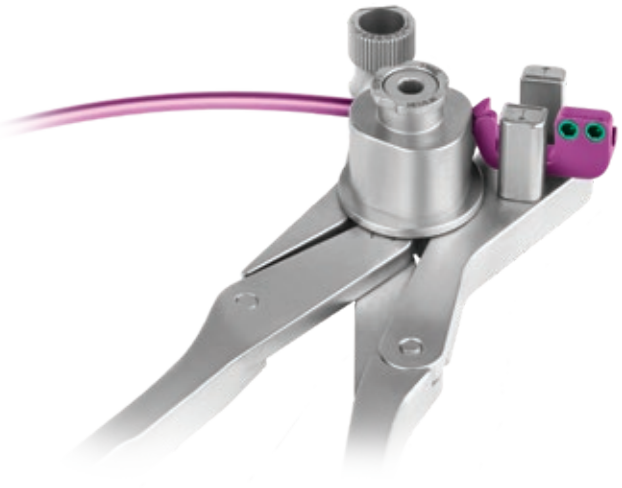

Using the REVERE® RESCUE® Bender

Before attaching the clamp to the existing hardware, use the **3.5mm Hex Driver, Self-Retaining** to back out the set screws from the clamp head. The bottom tip of each set screw should be level with the inferior side of the implant to allow the rod to be seated. Take care when backing out the set screws as they can be separated from the clamp body.



REVERE® RESCUE® Clamp with secure set screws




REVERE® RESCUE® Clamp with screws backed out

The **Rod Holder** or **Rod Gripper** may be used to grasp the REVERE® RESCUE® Clamp for enhanced stability when inserting the clamp. The clamp's screw head opening should frame the existing pedicle screw head and be positioned to fully engage the existing rod. The implant's integrated rod extends the construct to the desired level. Ensure that the contoured outgoing rod matches the anatomical requirements and screws at each level. Cut the rod to the desired length.



REVERE® RESCUE® Clamp fully engaged with existing rod

Use the 3.5mm Hex Driver, Self-Retaining to provisionally tighten the clamp set screws by inserting the hex into the set screw and rotating clockwise. Ensure the hex is fully seated prior to tightening.

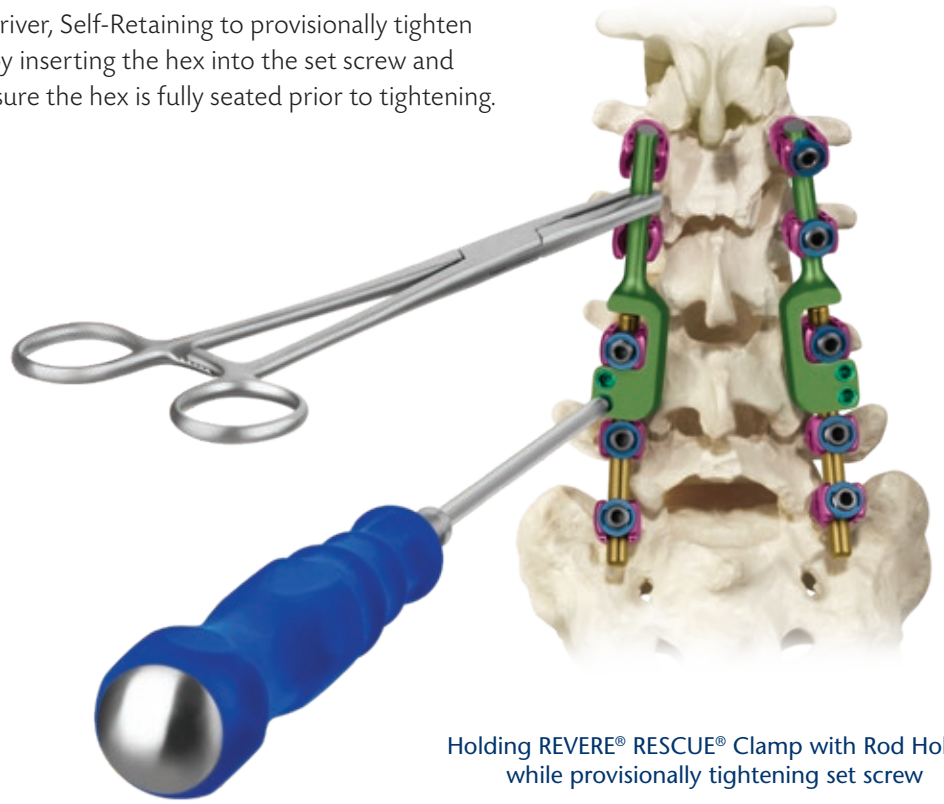

Holding REVERE® RESCUE® Clamp with Rod Holder while provisionally tightening set screw

Using the REVERE® RESCUE® Bender

Spread the handles of the REVERE® RESCUE® Bender until it is fully open.

1. Pull up the dial labeled Small, Medium, and Large and rotate to adjust the radius of curvature.

2. Position the clamp holder indicator arrows per the diagram at right for the desired bend.

3. Rotate the open/close dial to the open position so the flat surface is facing the rod. The rod can now be inserted into the bender. When the rod is in place, rotate the dial to the closed position to secure the rod.



Using the REVERE® RESCUE® Bender

To achieve the desired lordosis, kyphosis, lateral, and medial rod curvature for each clamp, position the clamp in the bender based on the images below.

After the clamp has been positioned correctly in the bender, contract the bender handles to curve the extension rod.

Additional bending along the rod portion should be accomplished using the standard Rod Bender.

In-Line Extension Clamp


Lordosis


Kyphosis


Lateral Bend


Medial Bend

Offset Extension Clamp


Lordosis


Kyphosis


Lateral Bend


Medial Bend

U-Connector


Lordosis


Kyphosis


Lateral Bend


Medial Bend


Implant Insertion (cont'd)

Rod-to-Rod Connector Insertion

Before attaching the connector to the existing implants, use the 3.5mm Hex Driver, Self-Retaining to back out the set screws from the connector head. The bottom tip of each set screw should be level with the bottom of the connector, so that the rod can be inserted without obstruction.


When an open connection point is selected, secure the open end onto the existing implants by placing the connector along the rod, in between the two screw heads. Provisionally tighten the engaged set screw using the 3.5mm Hex Driver, Self-Retaining.

Connectors have either open or closed connection points for the rod.



Open Clamp
Size specific to accomodate the existing REVERE®, CREO®, BEACON®, or PROTEX® rods.

Closed Connector
Sizes 5.5–6.0 (S)
5.5–6.5 (L)
can accomodate a range of rod diameters.

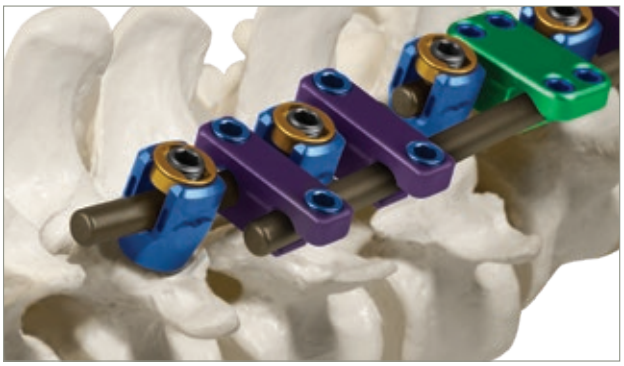

Open connection point secured onto rod

When a closed connection point is selected, it may be attached to a new rod in the construct by sliding the rod through the connector opening before attaching to the original rod. A closed connecter can also slide onto the end of the rod on the existing construct. Open-open clamps and single connectors must always be used in pairs.




Rod-to-Rod Connector placed on rod with additional opening



Closed connection point secured onto exisiting rod


Y Offset Connectors include two open connections and one closed connection. Align the screw head opening on the connector with the existing screw head. The two open connection points are placed along the existing rod. Slide the new rod into the closed connection point to extend the construct. If necessary, contour the outgoing rod *in situ* using the **Rod Benders, Left and Right**.

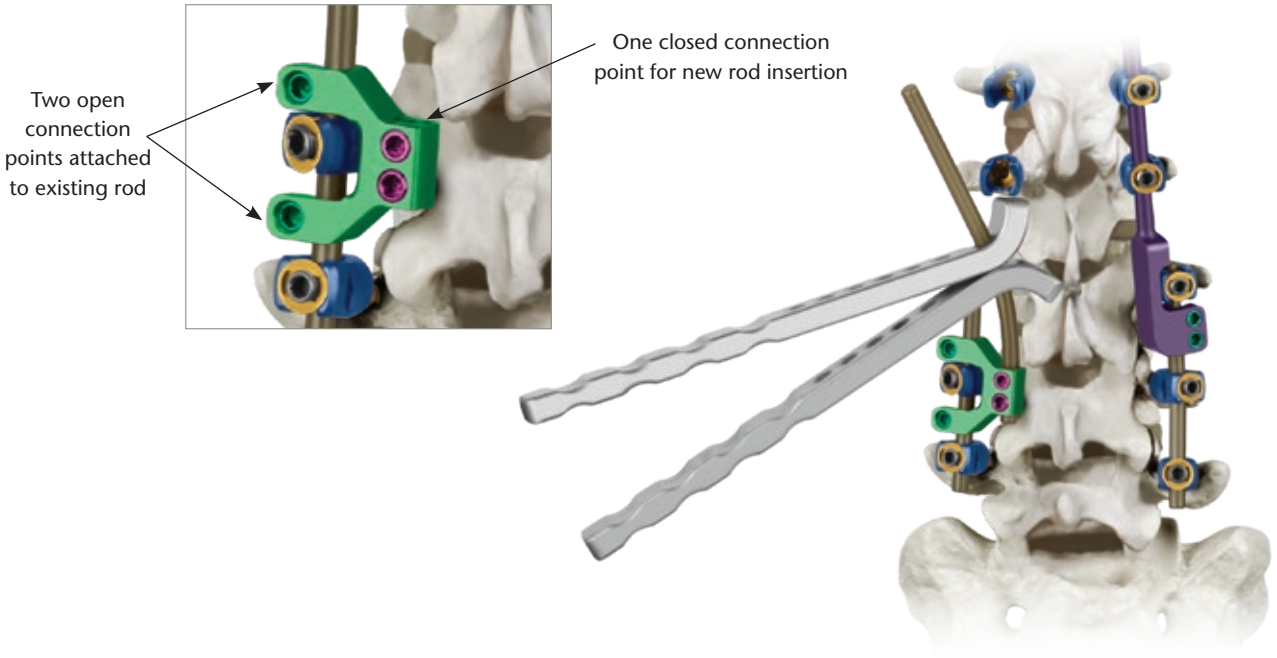

Contouring of outgoing rod using *in situ* Rod Benders, Left and Right

All Rod-to-Rod connectors may be used in conjunction with the REVERE® RESCUE® Clamps to enhance construct stability.


Use the 3.5mm Hex Driver, Self-Retaining, to provisionally tighten the connector set screws by inserting the hex into the set screw and rotating clockwise. Visually confirm the hex is fully seated before provisional tightening.

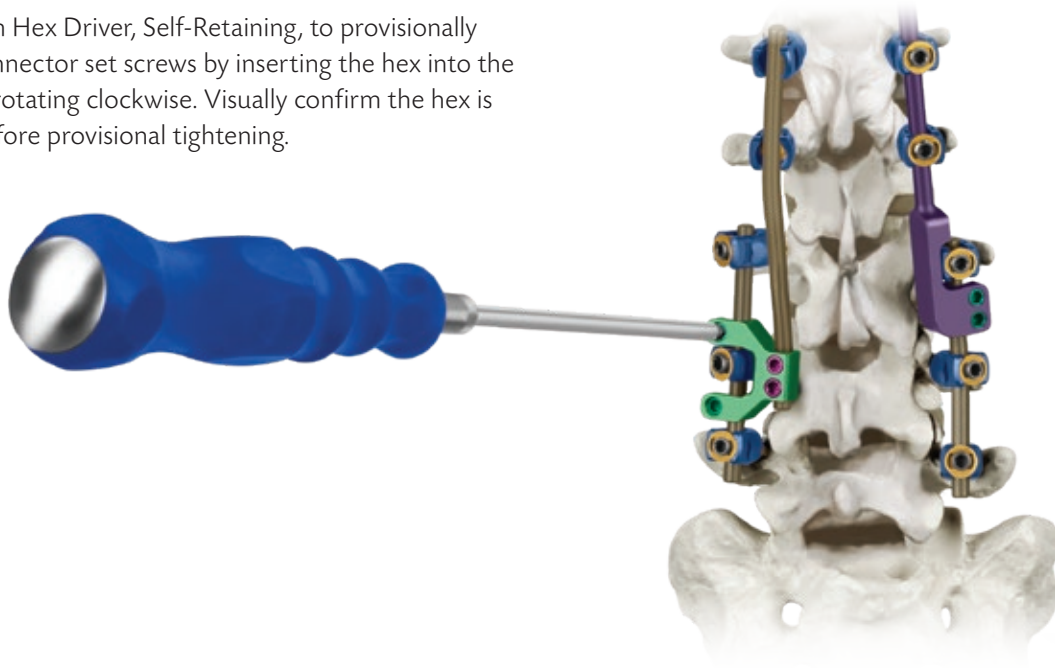


Hex driver fully seated prior to tightening

Step 6 Compression or Distraction

REVERE® pedicle screws can be compressed or distracted along the rod as necessary using the **Parallel Compressor** or **Distractor** respectively. REVERE® screws allow for screw angulation to be free or locked under compression or distraction. Tighten one of the set screws to establish a rigid point for compression or distraction. Once compression or distraction is completed, provisionally tighten the set screws using a 3.5mm hex driver.

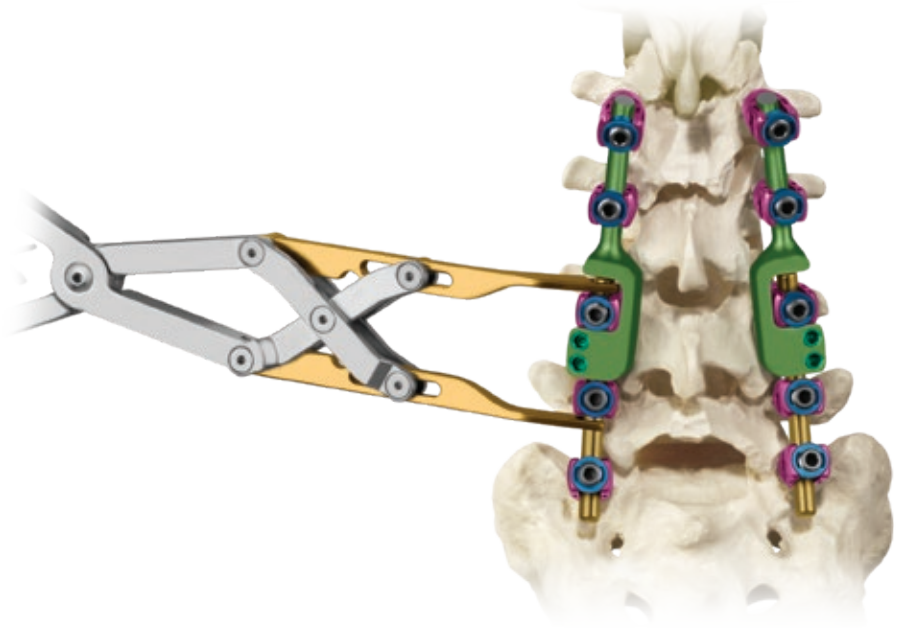

Compression

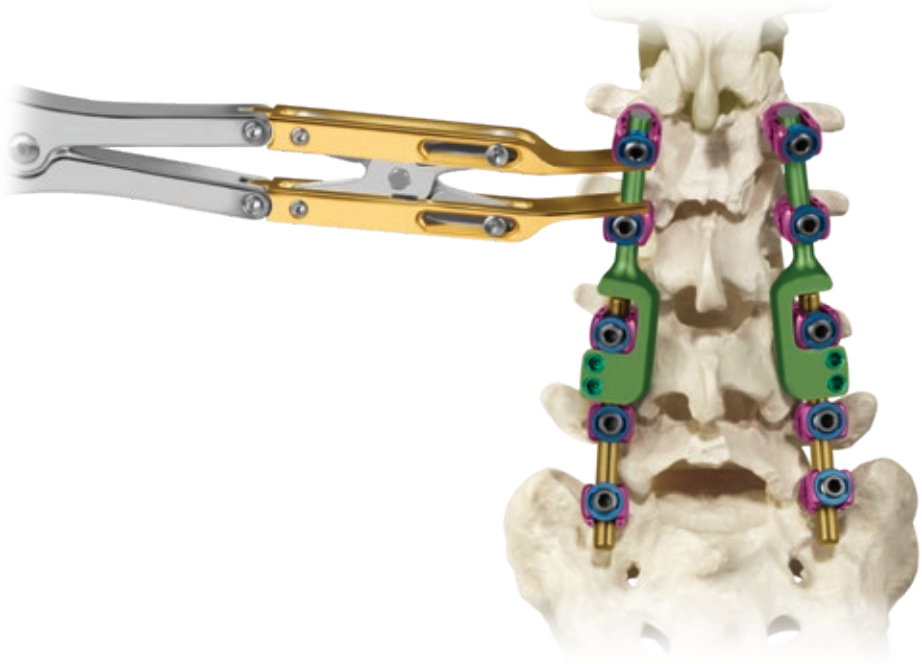


Distraction

Step 7 Final Tightening

Final tightening of the set screws is necessary to secure the construct and is accomplished using the **3.5mm Torque Limiting Hex Driver**.

Insert the hex driver into the set screw. Visually confirm that the hex is fully engaged in the set screw, perpendicular to the rod. Rotate the hex driver until it reaches the torque limit (5.5Nm) after two audible clicks. Repeat for all set screws.

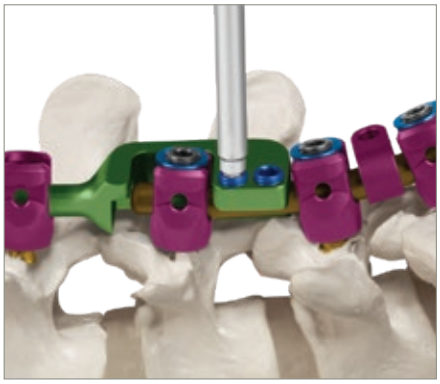

Hex fully engaged



Rotating the hex driver

Final Constructs








REVERE® RESCUE® Clamp construct









Y Offset Connector construct


REVERE® ADDITION® Revision System Connectors Guide


Part Number	Description	Compatible Rod Diameter Range and Rod Offset
102.965	In-Line Connector, 6.5–6.5mm	5.5–6.5mm 
124.980	In-Line Connector, 5.5–5.5mm	5.5–6.0mm 
124.962	Rod-to-Rod Clamp, 5.5–5.5mm	5.5–6.0mm  8mm, 12mm
124.963	Rod-to-Rod Clamp, 5.5–5.5mm, Wide	
154.758	Rod-to-Rod Clamp, 5.5–5.5mm, Single	5.5–6.0mm  12mm, 18mm
154.760	Rod-to-Rod Clamp, 5.5–5.5mm, 18mm Wide, Single	
154.862	Rod-to-Rod Clamp, 5.5–6.5mm	5.5–6.0mm 6.0–6.5mm  8mm, 12mm, 18mm
154.864	Rod-to-Rod Clamp, 5.5–6.5mm, Wide	
154.865	Rod-to-Rod Clamp Assembly, 5.5–6.5mm, 18mm Wide	
154.858	Rod-to-Rod Clamp, 6.5–6.5mm, Single	6.0–6.5mm  12mm, 18mm
154.860	Rod-to-Rod Clamp, 6.5–6.5mm, 18mm Wide, Single	
134.984	Rod-to-Rod Clamp, 6.35–6.35mm	6.0–6.5mm  8mm, 12mm, 18mm
134.985	Rod-to-Rod Clamp, 6.35–6.35mm, Wide	
134.986	Rod-to-Rod Clamp Assembly, 6.35–6.35mm, Extra Wide	
124.964	Parallel Connector Clamp, 5.5–5.5mm	5.5–6.0mm  8mm, 12mm
124.965	Parallel Connector Clamp, 5.5–5.5mm, Wide	
154.754	Parallel Connector Clamp, 5.5–6.5mm, Single	5.5–6.0mm, Open 5.5–6.5mm, Closed  12mm, 18mm
154.756	Parallel Connector Clamp, 5.5–6.5mm, 18mm Wide, Single	


REVERE® ADDITION® Revision System Connectors Guide

Part Number	Description	Compatible Rod Diameter Range and Rod Offset
154.854	Parallel Connector Clamp, 6.5–6.5mm, Single	6.0–6.5mm, Open 5.5–6.5mm, Closed  12mm, 18mm
154.856	Parallel Connector Clamp, 6.5–6.5mm, 18mm Wide, Single	
154.866	Parallel Connector Clamp, 6.5–6.5mm	6.0–6.5mm, Open 5.5–6.5mm, Closed  8mm, 12mm, 18mm
154.868	Parallel Connector Clamp, 6.5–6.5mm Wide	
154.869	Parallel Connector Clamp Assembly, 6.5–6.5mm, 18mm Wide	
102.971	Parallel Connector, 6.5–6.5mm	5.5–6.5mm  8mm, 12mm, 18mm
102.972	Parallel Connector, 6.5–6.5mm, Wide	
102.973	Parallel Connector, 6.5–6.5mm, Extra Wide	
102.981	Parallel Connector, Double, 6.5–6.5mm	5.5–6.5mm  8mm, 12mm, 18mm
102.982	Parallel Connector, Double, 6.5–6.5mm, Wide	
102.983	Parallel Connector, Double, 6.5–6.5mm, Extra Wide	
124.960	Parallel Connector, 5.5–5.5mm	5.5–6.0mm  8mm, 12mm
124.961	Parallel Connector, 5.5–5.5mm, Wide	
124.966	Parallel Connector, Double, 5.5–5.5mm	5.5–6.0mm  8mm, 12mm
124.967	Parallel Connector, Double, 5.5–5.5mm, Wide	
154.740	REVERE® Y Offset Connector, 5.5–6.0mm	5.5–6.0mm, Open 5.5–6.5mm, Closed  15mm
154.745	REVERE® Y Offset Connector, 6.0–6.35mm open, 5.5–6.5mm closed	6.0–6.5mm, Open 5.5–6.5mm, Closed  15mm

REVERE® ADDITION® REVISION SYSTEM SET

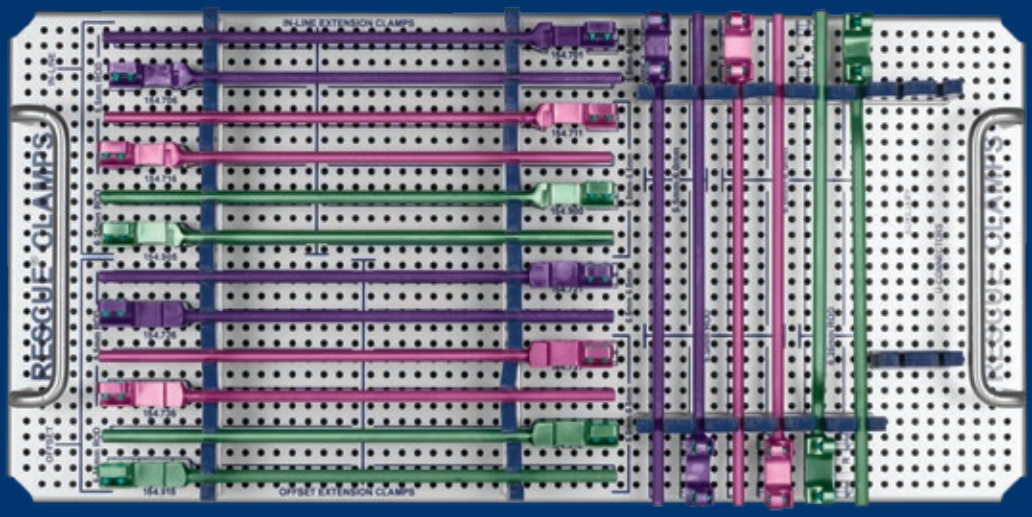

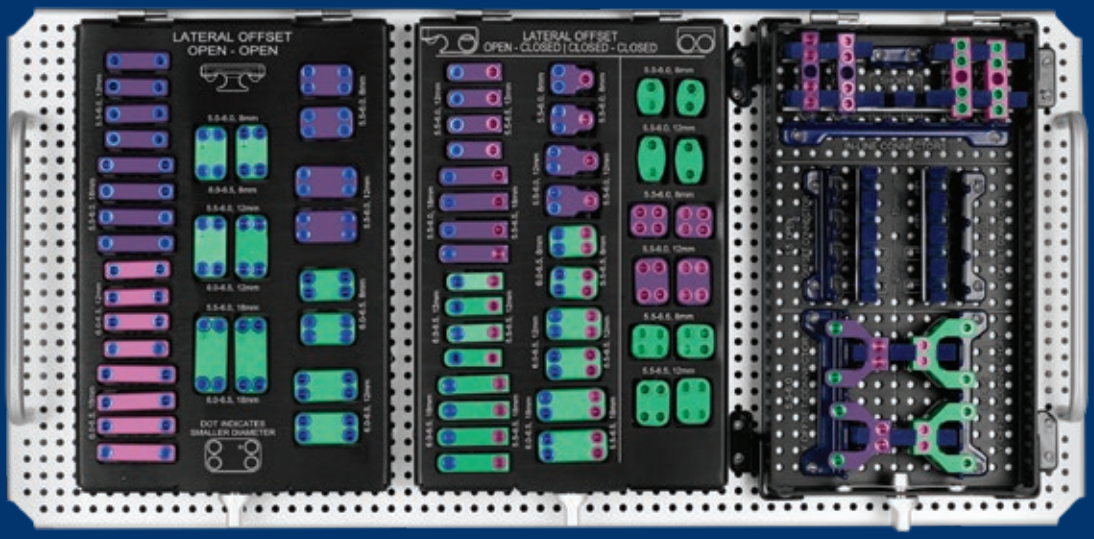

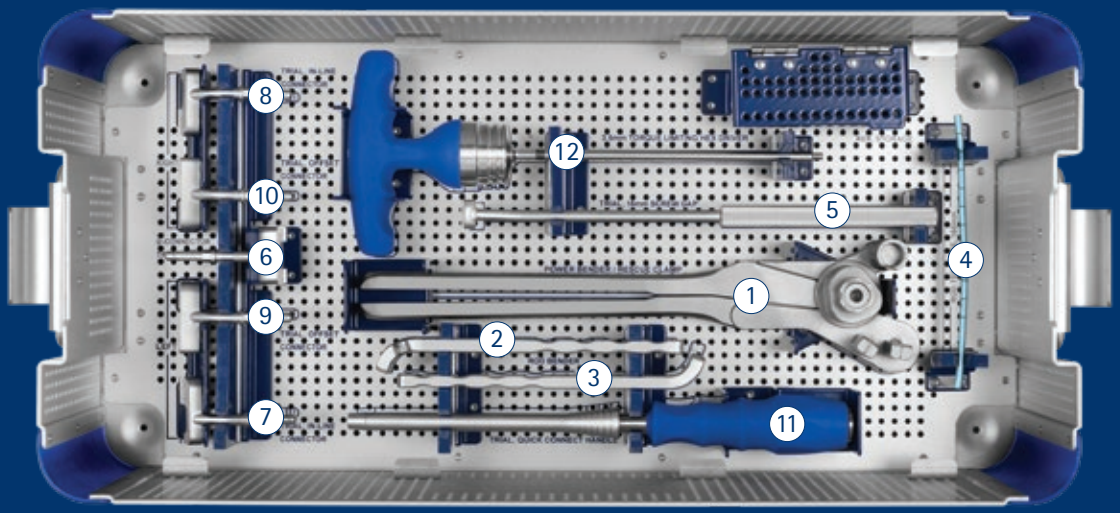

REVERE® ADDITION® Revision System Set 954.920

In-Line Connector		Qty
124.980	5.5–5.5mm	2
102.965	6.5–6.5mm	2

Parallel Connector Clamp		Qty
124.964	5.5–5.5mm	2
124.965	5.5–5.5mm, Wide	2
154.754	5.5–6.5mm, Single	4
154.756	5.5–6.5mm, 18mm Wide, Single	4
154.854	6.5–6.5mm, Single	4
154.856	6.5–6.5mm, 18mm Wide, Single	4
154.866	6.5–6.5mm	2
154.868	6.5–6.5mm Wide	2
154.869	6.5–6.5mm, 18mm Wide	2

Parallel Connector		Qty
124.960	5.5–5.5mm	0
124.961	5.5–5.5mm, Wide	0
102.971	6.5–6.5mm	2
102.972	6.5–6.5mm, Wide	2
102.973	6.5–6.5mm, Extra Wide	0
124.966	Double, 5.5–5.5mm	2
124.967	Double, 5.5–5.5mm, Wide	2
102.981	Double, 6.5–6.5mm	2
102.982	Double, 6.5–6.5mm, Wide	2
102.983	Double, 6.5–6.5mm, Extra Wide	0

Rod-to-Rod Clamp		Qty
124.962	5.5–5.5mm	2
124.963	5.5–5.5mm, Wide	2
154.758	5.5–5.5mm, Single	4
154.760	5.5–5.5mm, 18mm Wide, Single	4
154.862	5.5–6.5mm	2
154.864	5.5–6.5mm, Wide	2
154.865	5.5–6.5mm, 18mm Wide	2
134.984	6.35–6.35mm	2
134.985	6.35–6.35mm, Wide	2
134.986	6.35–6.35mm, Extra Wide	0
154.858	6.5–6.5mm, Single	4
154.860	6.5–6.5mm, 18mm Wide, Single	4

Y Offset Connector		Qty
154.740	5.5–6.0mm	2
154.745	6.0–6.5mm	2

In-Line Extension Clamp		Qty
154.701	5.5–6.0mm, 5.5mm Rod, Left, 200mm Length	1
154.706	5.5–6.0mm, 5.5mm Rod, Right, 200mm Length	1
154.711	6.0–6.5mm, 5.5mm rod, Left, 200mm Length	1
154.716	6.0–6.5mm, 5.5mm Rod, Right, 200mm Length	1
154.900	6.0–6.5mm, 6.35mm Rod, Left, 200mm Length	1
154.905	6.0–6.5mm, 6.35mm Rod, Right, 200mm Length	1


Offset Extension Clamp		Qty
154.721	5.5–6.0mm, 5.5mm Rod, Left, 200mm Length	1
154.726	5.5–6.0mm, 5.5mm Rod, Right, 200mm Length	1
154.731	6.0–6.5mm, 5.5mm Rod, Left, 200mm Length	1
154.736	6.0–6.5mm, 5.5mm Rod, Right, 200mm Length	1
154.910	6.0–6.5mm, 6.35mm Rod, Left, 200mm Length	1
154.915	6.0–6.5mm, 6.35mm Rod, Right, 200mm Length	1


U-Connector		Qty
154.850	5.5mm, 5.5mm Rod, 200mm Length, Right	1
154.851	5.5mm, 5.5mm Rod, 200mm Length, Left	1
154.852	6.35mm, 5.5mm Rod, 200mm Length, Right	1
154.853	6.35mm, 5.5mm Rod, 200mm Length, Left	1
154.950	6.35mm, 6.35mm Rod, 200mm Length, Right	1
154.955	6.35mm, 6.35mm Rod, 200mm Length, Left	1


NOTE: Set configuration may vary depending on location. Please consult your Globus Medical Sales Representative.

Items in gray are additionally available.

REVERE® ADDITION® REVISION SYSTEM SET (CONT'D)

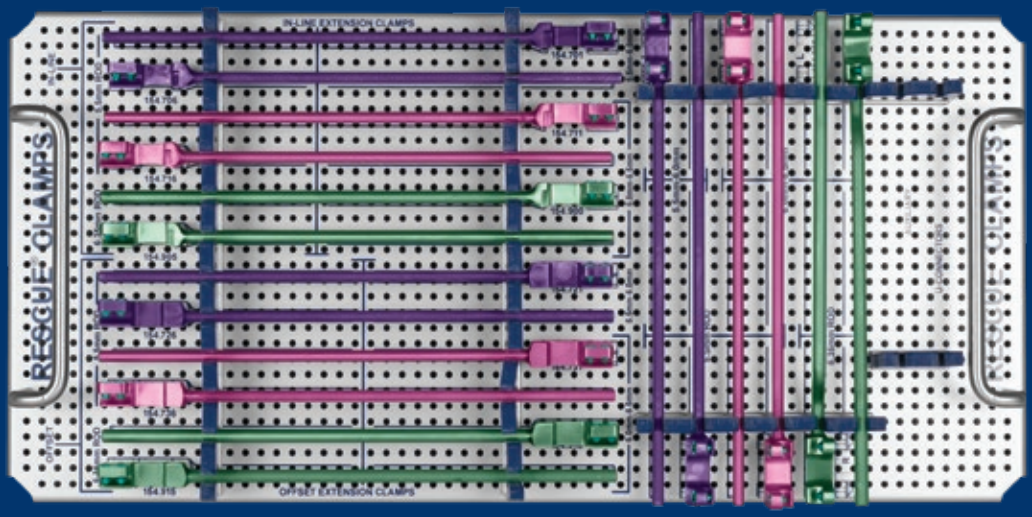

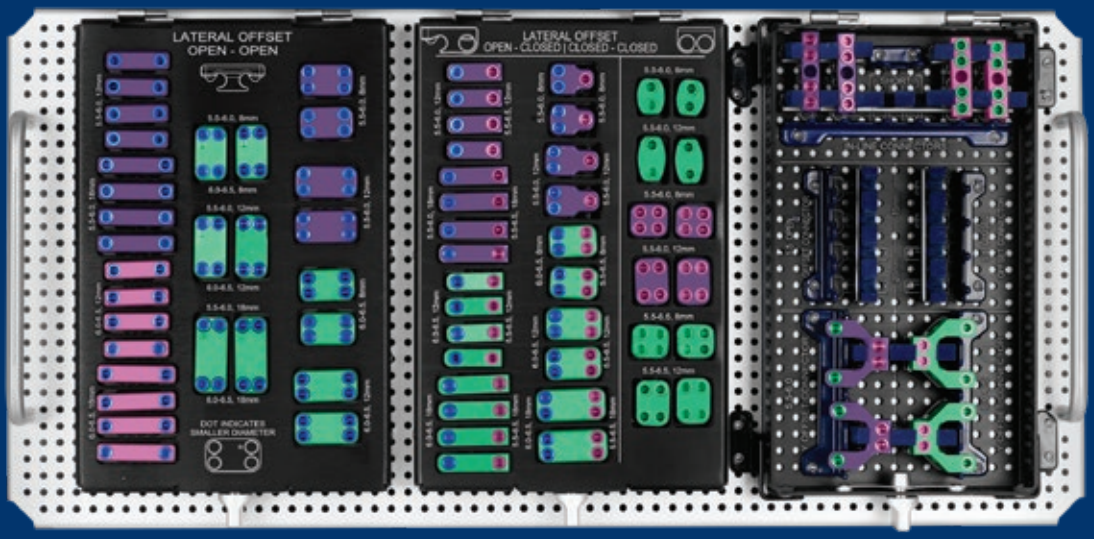

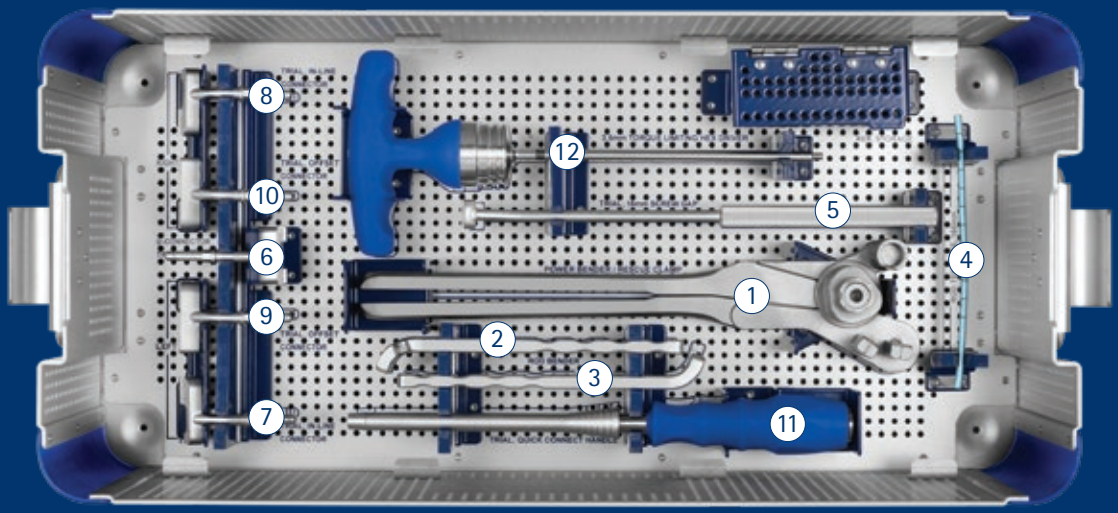

REVERE® ADDITION® Revision System Set 954.920 (Cont'd)


	Instruments		Qty
1	654.410	Rod Bender	1
2	652.690	Rod Bender, Left	1
3	652.691	Rod Bender, Right	1
4	602.501	Rod Template, 150mm	1
5	654.404	Trial, 15mm Screw Gap	1
6	654.405	Trial, U-Connector	1
7	654.406	Trial, In-Line Connector, Left	1
8	654.407	Trial, In-Line Connector, Right	1
9	654.408	Trial, Offset Connector, Left	1
10	654.409	Trial, Offset Connector, Right	1
11	654.411	Trial, Quick Connect Handle	1
12	654.415	3.5mm Torque Limiting Hex Driver	1
	954.010	Open-Open Connectors Module	
	954.011	Open-Closed and Closed-Closed Connectors Module	
	954.012	Inline, Sacral and Y Connectors Module	
	954.020	REVERE® ADDITION® Connectors Tray	
	954.210	REVERE® ADDITION® Revision Graphic Case	
	924.910LN	REVERE® ADDITION® Revision Fixation System - TAV Loaner Set	


Additionally Available Instruments


602.508	Rod Cutter
602.522	Rod Gripper
624.406	3.5mm Hex Driver, Self-Retaining
624.503	Rod Compressor
624.504	Rod Distractor
624.510	Rod Holder

NOTE: Set configuration may vary depending on location. Please consult your Globus Medical Sales Representative.

REVERE® ADDITION® REVISION SYSTEM STAINLESS STEEL SET

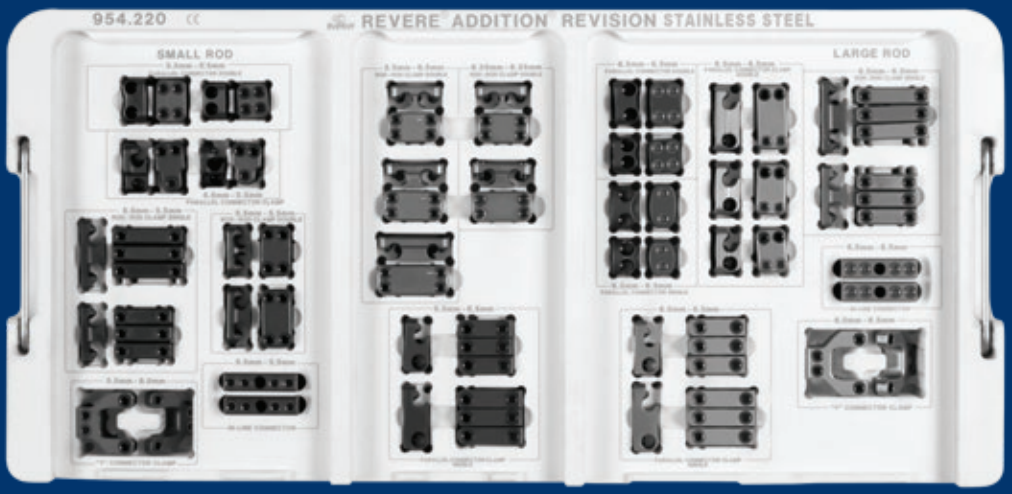

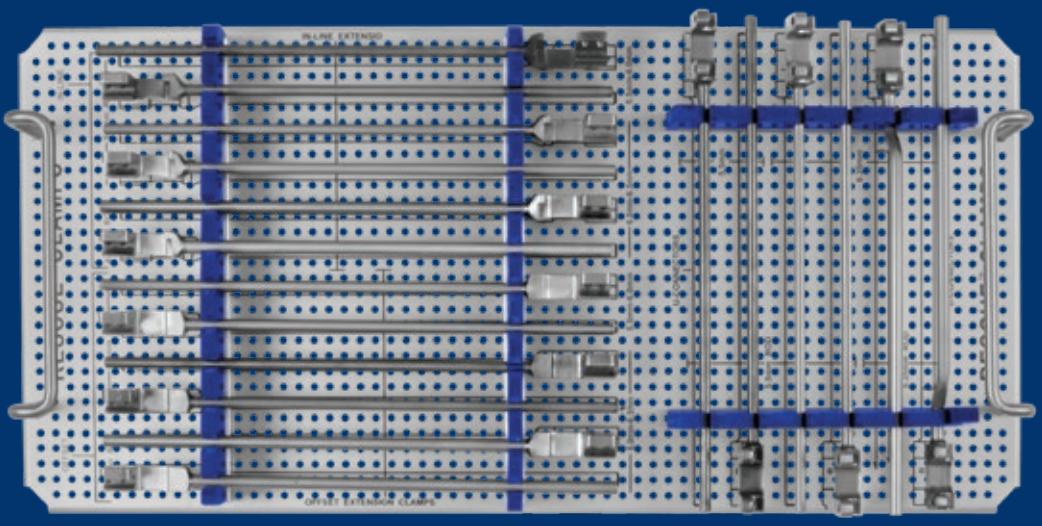

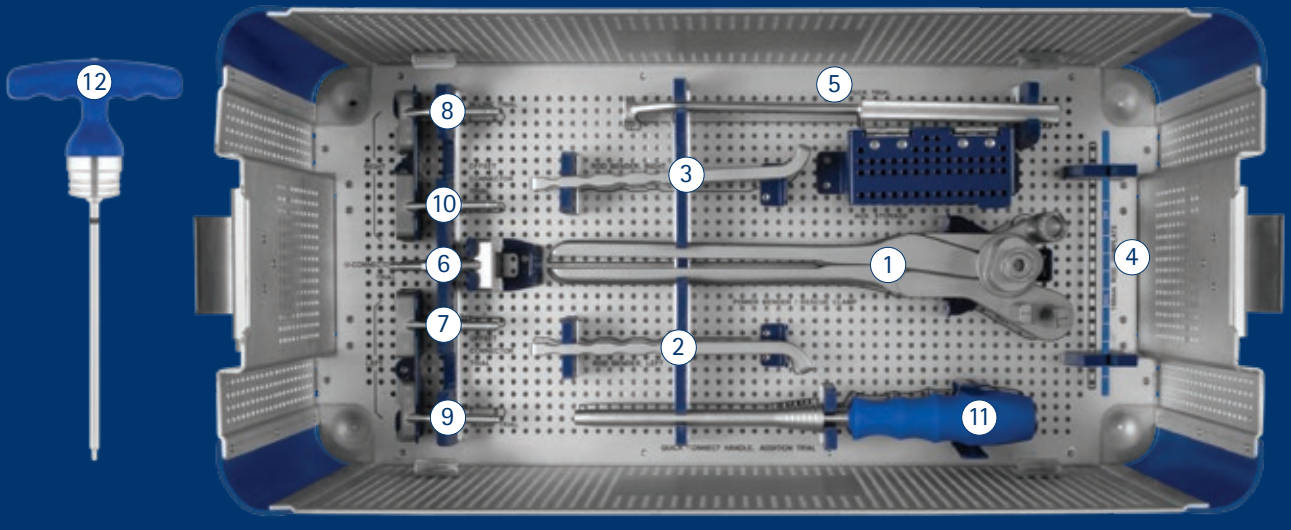

REVERE® ADDITION® Revision System
Stainless Steel Set 954.912

SS In-Line Connector		Qty
224.980	5.5–5.5mm	2
254.965	6.5–6.5mm	2

SS Parallel Connector Clamp		Qty
224.964	5.5–5.5mm	2
224.965	5.5–5.5mm, Wide	2
254.754	5.5–6.5mm, Single	4
254.756	5.5–6.5mm, 18mm Wide, Single	4
254.854	6.5–6.5mm, Single	4
254.856	6.5–6.5mm, 18mm Wide, Single	4
254.866	6.5–6.5mm	2
254.868	6.5–6.5mm Wide	2
254.869	6.5–6.5mm, 18mm Wide	2

SS Parallel Connector		Qty
224.960	5.5–5.5mm	
224.961	5.5–5.5mm, Wide	
234.960	6.35–6.35mm	2
234.961	6.35–6.35mm, Wide	2
234.962	6.35–6.35mm, Extra Wide	
234.964	6.35–6.35mm, Wide	2
224.966	Double, 5.5–5.5mm	2
224.967	Double, 5.5–5.5mm, Wide	2
234.963	Double, 6.35–6.35mm	2
234.965	Double, 6.35–6.35mm, Extra Wide	

SS Rod-to-Rod Clamp		Qty
224.962	5.5–5.5mm	2
224.963	5.5–5.5mm, Wide	2
254.758	5.5–5.5mm, Single	4
254.760	5.5–5.5mm, 18mm Wide, Single	4
254.862	5.5–6.5mm	2
254.864	5.5–6.5mm, Wide	2
254.865	5.5–6.5mm, 18mm Wide	2
234.984	6.35–6.35mm	2
234.985	6.35–6.35mm, Wide	2
234.986	6.35–6.35mm, Extra Wide	
254.858	6.5–6.5mm, Single	4
254.860	6.5–6.5mm, 18mm Wide, Single	4

SS Y Offset Connector		Qty
254.740	5.5–6.0mm	2
254.745	6.0–6.5mm	2

NOTE: Set configuration may vary depending on location. Please consult your Globus Medical Sales Representative.

Items in gray are additionally available.

SS In-Line Extension Clamp		Qty
254.700	5.5–6.0mm, 5.5mm Rod, Left, 200mm Length	1
254.705	5.5–6.0mm, 5.5mm Rod, Right, 200mm Length	1
254.710	6.0–6.5mm, 5.5mm Rod, Left, 200mm Length	1
254.715	6.0–6.5mm, 5.5mm Rod, Right, 200mm Length	1
254.900	6.0–6.5mm, 6.35mm Rod, Left, 200mm Length	1
254.905	6.0–6.5mm, 6.35mm Rod, Right, 200mm Length	1

SS Offset Extension Clamp		Qty
254.720	5.5–6.0mm, 5.5mm Rod, Left, 200mm Length	1
254.725	5.5–6.0mm, 5.5mm Rod, Right, 200mm Length	1
254.730	6.0–6.5mm, 5.5mm Rod, Left, 200mm Length	1
254.735	6.0–6.5mm, 5.5mm Rod, Right, 200mm Length	1
254.910	6.0–6.5mm, 6.35mm Rod, Left, 200mm Length	1
254.915	6.0–6.5mm, 6.35mm Rod, Right, 200mm Length	1

SS U-Connector		Qty
254.850	5.5mm, 5.5mm Rod, Right, 200mm Length	1
254.851	5.5mm, 5.5mm Rod, Left, 200mm Length	1
254.852	6.35mm, 5.5mm Rod, Right, 200mm Length	1
254.853	6.35mm, 5.5mm Rod, Left, 200mm Length	1
254.950	6.35mm, 6.35mm Rod, Right, 200mm Length	1
254.955	6.35mm, 6.35mm Rod, Left, 200mm Length	1

	Instruments		Qty
1	654.410	Rod Bender	1
2	652.690	Rod Bender, Left	1
3	652.691	Rod Bender, Right	1
4	602.501	Rod Template, 150mm	1
5	654.404	Trial, 15mm Screw Gap	1
6	654.405	Trial, U-Connector	1
7	654.406	Trial, In-Line Connector, Left	1
8	654.407	Trial, In-Line Connector, Right	1
9	654.408	Trial, Offset Connector, Left	1
10	654.409	Trial, Offset Connector, Right	1
11	654.411	Trial, Quick Connect Handle	1
12	654.415	3.5mm Torque Limiting Hex Driver	1
	954.222	REVERE® ADDITION® Revision Module Assembly, Stainless Steel	
	954.212	Stainless Steel REVERE® ADDITION® Revision Graphic Case	

Notes

Notes

Globus Medical
Valley Forge Business Center
2560 General Armistead Avenue
Audubon, PA 19403
www.globusmedical.com

Customer Service:
Phone 1-866-GLOBUS1 (or 1-866-456-2871)
Fax 1-866-GLOBUS3 (or 1-866-456-2873)

©2023 Globus Medical. All rights reserved. Patent www.globusmedical.com/patents. Life moves us is a registered trademark of Globus Medical. Please refer to package insert for description, indications, contraindications, warnings, precautions and other important information.

EC REP : AJW Technology Consulting GmbH
Breite Straße 3 40213 Düsseldorf, Germany

CE 0297

GMTGD630U
10.23 RevB