Auxein

SUPRAPATELLAR INSTRUMENTATION FOR EXPERT TIBIAL NAIL

Surgical Technique

NEXT-LEVEL CARE

ABOUT US

Auxein Medical is an integrated, research based, orthopaedic implants & instruments manufacturing company, producing a wide range of quality, affordable generic implants, trusted by healthcare professionals and patients across geographies. It is the Company's constant endeavour to provide a wide basket of generic and our innovator products that exceed the highest expectations of customers in term of quality and safety. The company has world-class manufacturing unit established in India and serves customers in over 75 countries worldwide.

IMPACTING HEALTHCARE GLOBALLY

Our Reach & Influence

500+
Employees Worldwide

75+
Operations in Countries

150+
Distributors Worldwide

20M+
Patients Cured

200+
FDA Approved Products

250+
Machines Worldwide

3000+
Products Orthopedic Solutions

Auxein is dedicated to advancing medical technology through innovative orthopedic solutions, including **Trauma, Arthroscopy, and Reconstructive Procedures**, with a commitment to improving patient outcomes worldwide. Our approach integrates advanced research, precision engineering, and high-quality manufacturing to develop reliable implants and surgical instruments that address the evolving needs of modern orthopedic practice.

OUR ACHIEVEMENTS



OVER THE YEARS

Disclaimer: Not all products in this catalogue are covered by European CE, US FDA, or other certifications. Please contact our Sales Team for product-specific certification details.


HAAS
HAAS
POWER ON
POWER OFF
EMERGENCY STOP
HANDLE JOG
RESET
F1
F2
F3
F4
OVERRIDES
CYCLE START
STOP
REV
SPINDLE



At Auxein, it is our goal to provide the best in class quality and value to every individual. Consistency is a virtue we pursue with a passion. From the procurement of raw materials to the manufacturing of our range of 1200+ orthopaedic implant products, we employee world-class systems and technology at par with the highest standards of globally recognized evaluation systems. The Expert Tibia Nailing Suprapatellar Insertion System is part of our orthopedic trauma portfolio designed for the intramedullary fixation of tibial fractures. Developed with input from global experts, the system provides reliable stabilization to help achieve stable fixation, optimal load sharing, and accurate anatomical alignment during fracture management.

Suprapatellar Instrumentation for Expert Tibial Nail

Expert Tibia Nailing System

Introduction


The Expert Tibia Nailing System is designed to expand the range of tibial fractures that can be treated with intramedullary fixation. The system is intended for the management of diaphyseal, metaphyseal, and selected intra-articular fractures of the proximal and distal tibia. The nail design enhances the stability of the bone–implant construct and helps reduce the risk of secondary malalignment.
Multiple multidirectional interlocking screw options allow secure fixation and improved stability, particularly in short proximal or distal tibial segments. The end cap mechanism provides additional angular stability between the proximal oblique screw and the nail, contributing to reliable fracture stabilization and maintenance of alignment.

Locking Options

Proximal Segment Fractures: For proximal fractures, locking the nail with the knee in extension is recommended. This helps neutralize deforming forces on the proximal fragment caused by the quadriceps mechanism and reduces soft tissue pressure associated with nail insertion instruments. The extended position also facilitates accurate assessment of rotational alignment prior to final locking.

Diaphyseal Segment Fractures: For diaphyseal fractures, distal locking is generally performed first to allow intraoperative compression and stabilization of the fracture.


Distal Segment Fractures: For distal tibial fractures, distal locking is recommended initially to facilitate fracture reduction and stabilization before completing proximal locking.

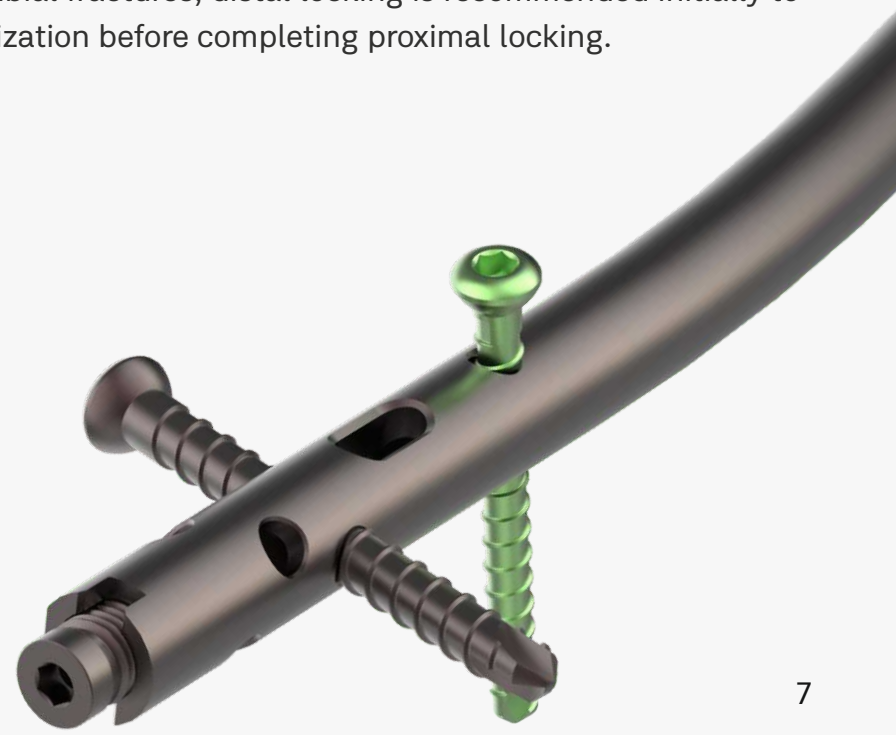

Indications:

The Expert Tibia Nail is indicated for the treatment of tibial shaft fractures, as well as metaphyseal and selected intra-articular fractures of the proximal and distal tibia. These include:

- Proximal tibial fractures – AO/OTA 41-A2, 41-A3.
- Tibial shaft fractures – all diaphyseal fracture patterns.
- Distal tibial fractures (pilon type) – AO/OTA 43-A1, 43-A2, 43-A3.
- Combined fracture patterns involving the tibial shaft and metaphyseal regions.

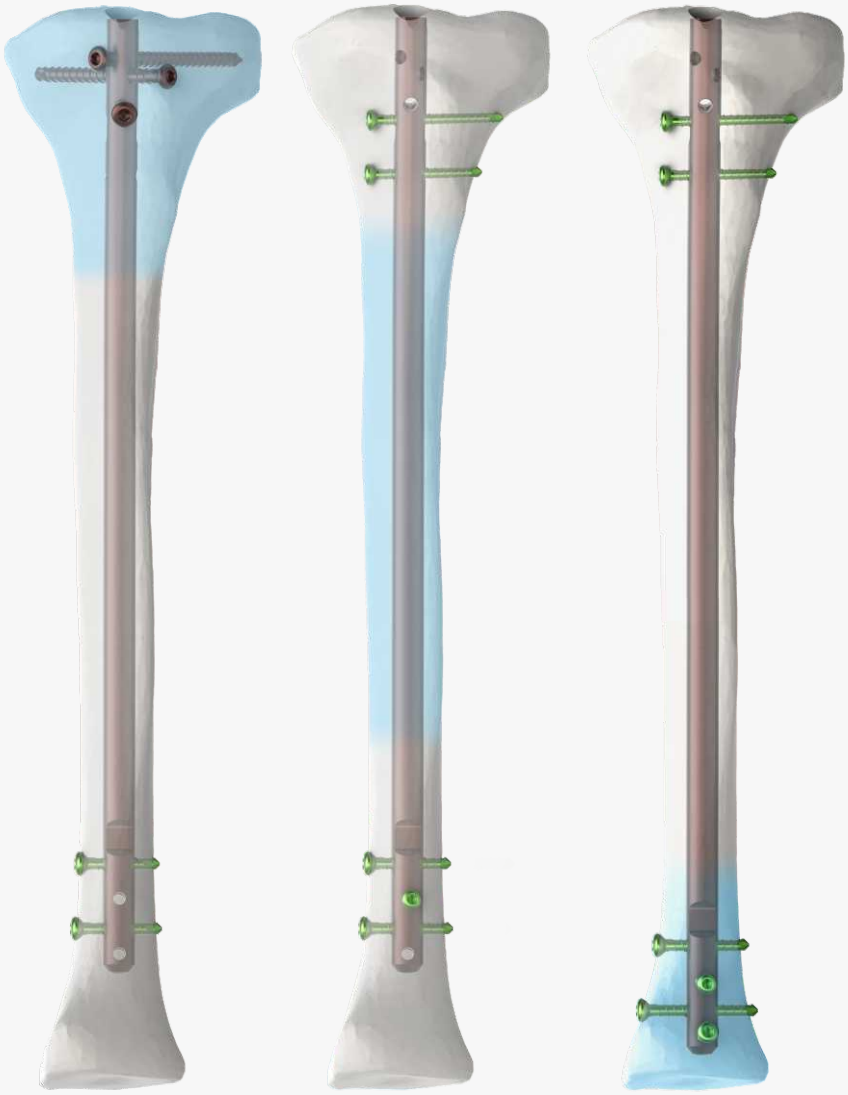

The system is intended to provide stable intramedullary fixation and maintenance of anatomical alignment during fracture management.

PRODUCT SPECIFICATIONS:

Expert Tibial Nail

Diameters:
Ø8mm, Ø9mm, Ø10mm, Ø11mm & Ø12mm

Length:
255mm - 375mm (With 15mm difference)

Available In:
Stainless Steel and Titanium

Color Coding *(only for Titanium) :*
Type-II For Expert Tibia Nail

Cannulation:

All Expert Tibia Nails are cannulated which enables nail insertion over guide wire for reamed or unreamed techniques.

The ball tip guide wires may be removed through the nail and insertion handle assembly (no exchange tube required).

Advanced Nail Design:

- Anatomical proximal bend designed to facilitate easier nail insertion and improved alignment during implantation.
- Two advanced medio-lateral (ML) locking options allowing primary compression or secondary controlled dynamization.
- Multiple distal locking options, including two medio-lateral (ML) and one anteroposterior (AP) locking holes, to enhance stability of the distal fragment.



Important: Solid Nail for unreamed technique are also available on special request

End Cap For Expert Tibia Nail

Length:
0mm, 5mm, 10mm and 15mm

Available in:
Stainless Steel and Titanium

Color coding *(only for Titanium) :*
Type-II For End Cap



Features:

- End Cap prevents ingrowth of hard & soft tissue which facilitates nail extraction.
- 0mm End Cap sits flush with nail.
- End Cap with different option of length can extend nail height if nail is over inserted.
- Securely lock the most proximal oblique locking screw to create a fixed-angle construct.
- Cannulated.

Ø4.8mm Locking Bolt, Self-Tapping, For Expert Tibia Nail

Length:
25mm - 90mm (With 5mm difference)

Available in:
Stainless Steel and Titanium

Color Coding *(only for Titanium) :*
Type-II For Ø4.8mm Locking Bolt



Ø4.4mm Locking Bolt, Self-Tapping, For Expert Tibia Nail


Length:
24mm - 88mm (With 2mm difference)

Available in:
Stainless Steel and Titanium

Color Coding *(only for Titanium) :*
Green For Ø4.4mm Locking Bolt


Features:

- Thread closer to screw head for better and improved stability
- Self Tapping
- Hex head
- Larger cross section for improved mechanical resistance.

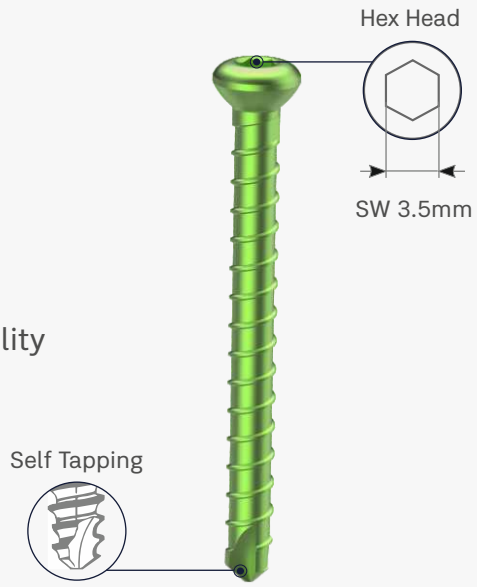

Entry Point:

The entry point defines the optimal position of the Expert Tibial Nail in the intramedullary canal. This is more important for proximal and distal third fractures to prevent fragment displacement.

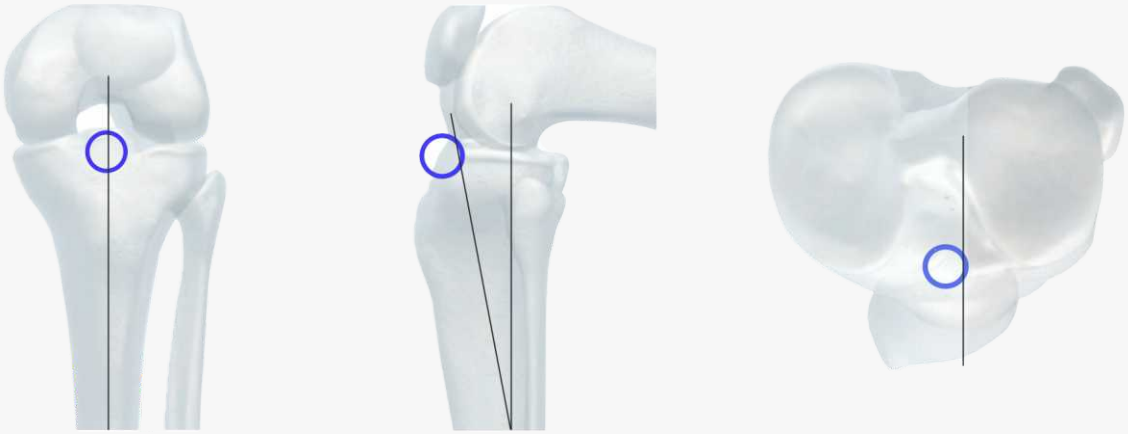


In anterior - posterior (AP) view the entry point is in line with the axis of the intra-medullary canal and with the lateral tubercle of the inter-condylar eminence.

In lateral view the entry point is at the ventral edge of the tibial plateau.


Opening The Tibia

1. Position patient

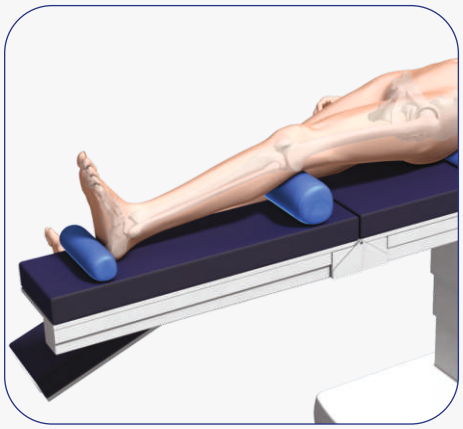

Position the patient supine on the radiolucent table. Ensure that the knee of the injured leg can be flexed 10° – 20°. Position the image intensifier so that visualization of the tibia, including the articular surface proximally and distally, is possible in AP and lateral views.
The knee roll can be placed under the lower part of the thigh if it obstructs the view of the tibial plateau in the AP view.

2. Reduce fracture

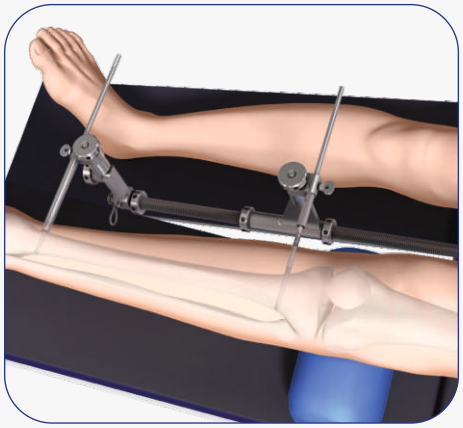

Perform closed reduction manually by axial traction under image intensifier. The use of the Large Distractor may be appropriate in certain circumstances where part of the thigh if it obstructs the view of the tibial plateau in the AP view.
Notes:
The reduction can be temporarily fixed with reduction clamps. In epiphyseal fractures, the condyles or the pilon are fixed first in order to enable the nail insertion.

3. Measuring Nail length and diameter:

The C-Arm is positioned in such a way to get AP view of the Distal Tibia. The Radiographic ruler **(7-112-24)** is held parallel to the Tibia bone. The ruler is adjusted until the distal end of ruler is aligned with the desired nail insertion depth.

After finalizing the position of radiographic ruler, the C-Arm is moved to the Proximal Tibia to take an image in AP view. The length of the nail is determined from reading on the ruler pointing in level or just below the tibial plateau.




Under C-Arm, the diameter gauge part of the radiographic ruler is placed over the narrowest part of the Tibia medullary canal in either AP or lateral view. The reading on the diameter gauge coinciding with the canal width is chosen.


Note: All the readings are to be taken only after the compression of the bone has been achieved. As an alternative, these readings can be measured from the uninjured Tibia bone.

4. Entry Point

With the knee in full extension, make a 2–4 cm longitudinal skin incision 4 cm proximal to the superior pole of the patella. The deep incision, also longitudinal, splits the quadriceps tendon in its midsubstance, just above its insertion into the patella and enters the knee joint through the suprapatellar pouch. Blunt dissection can be used to loosen the patella in the suprapatellar pouch, allowing the patella to lift off. Displace the patella anteriorly.
The entry point defines the optimal position of the Expert Tibial Nail in the intramedullary canal. This is more
important for proximal and distal third fractures to prevent fragment displacement.



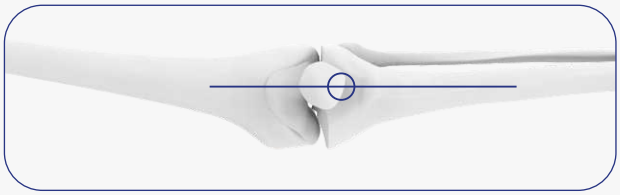

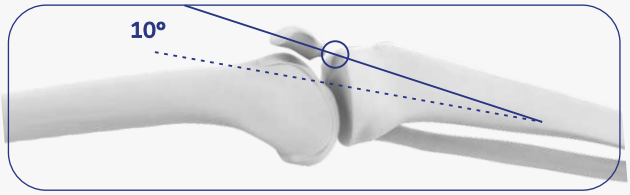


In anterior - posterior (AP) view the entry point is in line with the axis of the intra-medullary canal and with the lateral tubercle of the inter-condylar eminence.

In lateral view the entry point is at the ventral edge of the tibial plateau.

5. Insert protection sleeves

7-112-02	Protection Sleeve Handle
7-112-03	Outer Protection Sleeve
7-112-04	Protection Sleeve 16/14.5mm
7-112-05	Trocar Ø14.5mm, PEEK

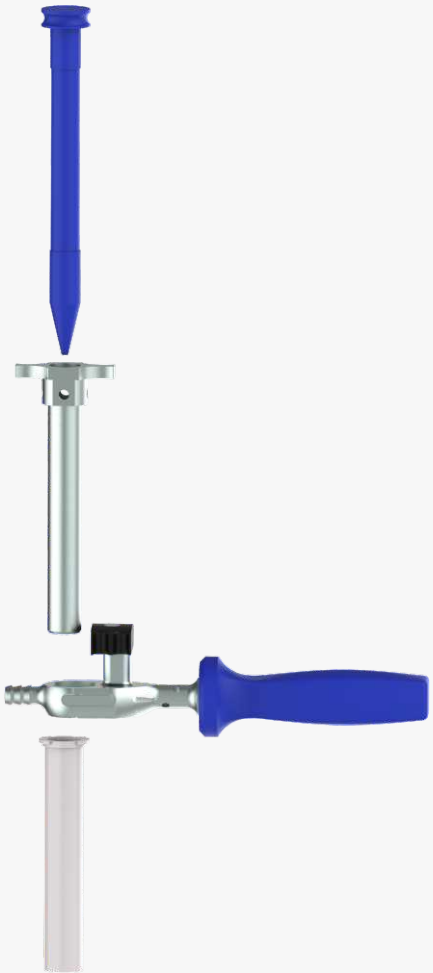

5. Insert protection sleeves




Assemble the handle, inner protection sleeve, outer protection sleeve, and trocar. Rotate the knob to lock the assembly into the handle during insertion.

Insert the handle assembly through the incision into the knee joint, so that it glides between the articular surface of the patella and the trochlea of the distal femur and rests securely in this groove, while the patella is displaced anteriorly above the cannula. When the trocar reaches the surface of the tibia, rotate the knob on the handle to allow the trocar to slide out, as the cannula is advanced to the anterior surface of the proximal tibia. Remove the trocar.

Precaution: The knee must remain in extension once the handle assembly has been inserted.

6. Insert guide wire

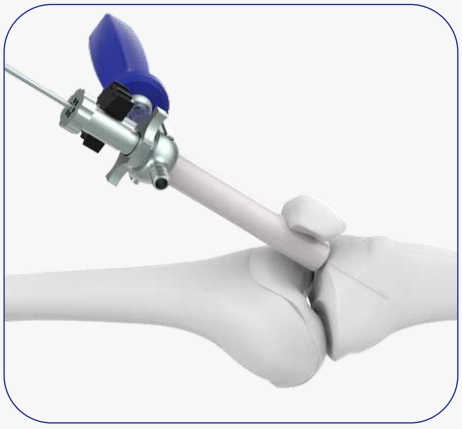

After removal of the trocar, insert the centering sleeve **(7-112 06)** through the inner protection sleeve.


Advance to the anterior surface of the tibia. Slight adjustment of the knee flexion (between 10° and 20°) will provide the ideal radiographic location for the starting point and insertion of a guide wire. Insert the guide wire approximately 8cm–10cm and check the position under imaging in the AP and lateral views.

Adjustments to the guide wire **(520-013)** location can be “dialed-in” by rotating the centering sleeve to place a second guide wire while the first guide wire remains in place.

After correct placement of the second guide wire, remove the initial guide wire and centering sleeve.

7. Anchor handle for protection sleeves

Use a 3.2 mm guide wire to anchor the handle assembly to the femoral condyles and maintain the position of the handle assembly during the procedure. This anchor prevents the cannula from backing out and off of the tibia.

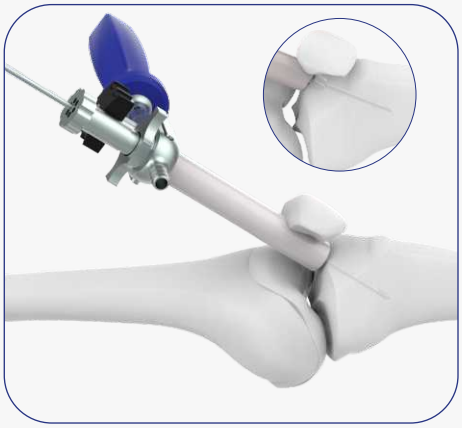

8. Open medullary canal

Place the drill bit **(520-004)** Guide Wire With Threaded Tip Ø3.2mm x Thread Length 10mm x Length 300mm over the guide wire, through the inner protection sleeve, and down to the bone. Drill to a depth of approximately 8cm–10cm. The guide wire and drill bit should not reach the posterior cortex. Remove the drill bit and guide wire.

Precaution: Dispose of the guide wire. Do not reuse.

Reaming (optional)

Precaution: Do not ream without the inner protection sleeve in place to protect the outer protection sleeve.



Inserting the reaming rod
Insert the 2.5 mm reaming rod with ball tip and extension into the medullary canal to the desired insertion depth.

Ream
Starting with the 8.5mm diameter reaming head, ream to a diameter of 0.50mm-1.0mm greater than the nail diameter. Ream in 0.5mm increments and advance the reamer with steady, moderate pressure. Do not force the reamer. Partially retract the reamer often to clear debris from the medullary canal.

The reamer can catch on the edge of the inner protection sleeve because of the sharp angle entering the tibia (1). Stop reamer rotation and lift up on the drill to center the reamer shaft in the sleeve (2). Move the reamer in and out until the reamer comes out.



Instruments:


7-112-02	Protection Sleeve Handle for Expert Tibia Nail - Suprapatellar Insertion



7-112-03	Outer Protection Sleeve for Expert Tibia Nail - Suprapatellar Insertion



7-112-04	Protection Sleeve 16/14.5mm for Expert Tibia Nail - Suprapatellar Insertion

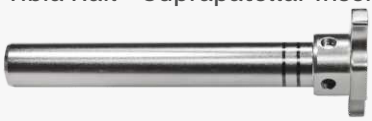

7-112-26	Quick Coupling T Handle for Expert Tibia Nail - Suprapatellar Insertion



7-112-30	Flexible Reamer Shaft (Jacob Connection) for Expert Tibia Nail - Suprapatellar Insertion



7-112-40	Reamer Head



520-058	Guide wire without Ball Tip Ø2.5mm x Length 1000mm - Nitinol, for Expert Tibia Nail



Inserting the Nail

1. Assemble insertion instruments

Orient the insertion handle anteriorly, and match the tang on the handle to the notch in the nail.

Place the connecting screw into the insertion handle and thread it into the proximal nail end, using the rod pusher for reaming rod.

Verify the nail is oriented properly on the insertion handle; secure the assembly with the screwdriver

Alternatively. secure the assembly using the screwdriver.

Remove the inner protection sleeve from the handle for protection sleeves.

When removing the inner protection sleeve, lift or rotate handle to gain access to the lower lever lock. Depress both upper and lower lever locks and slide the inner protection sleeve out.



7-112-01	Insertion Handle for Expert Tibia Nail - Suprapatellar Insertion



7-112-19	Nail Holding Bolt, Long, for Expert Tibia Nail - Suprapatellar Insertion



7-112-46	Allen Key, Hex 5mm for Expert Tibia Nail (Suprapatellar Insertion)




2. Insert nail

Ensure inner protection sleeve is removed.

Insert the nail into the intramedullary canal. Use a twisting motion to advance the nail.

- Monitor the nail passage across the fracture; control in two planes to avoid malalignment
- Insert the nail until it is at or below the tibial opening. Check final nail position in AP and lateral views.

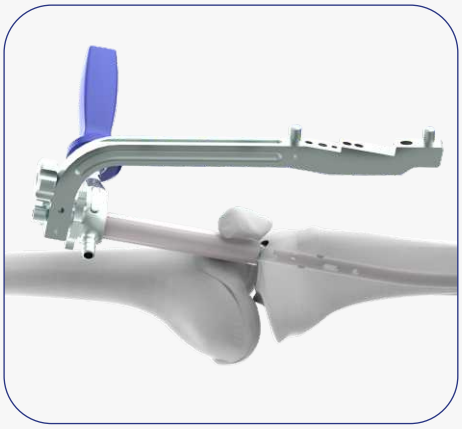


Note:

For proximal locking, mount the aiming arm only when the tibial nail has been completely inserted, otherwise the aiming arm may loosen during nail insertion.

Optional instruments

If needed, use light, controlled Sliding Hammer for Expert Tibia Nail - Suprapatellar Insertion **(7-112-21)** blows to seat the nail. Thread the Hammer Guide Shaft for Expert Tibia Nail - Suprapatellar Insertion **(7-112-22)** into the insertion handle along with the Nut for Hammer Guide Shaft **(7-112-23)** and secure it, using the 11 mm combination wrench. Lock the head of the hammer in place by tightening the nut onto the threads located below the hammer head, using the 4.5 mm pin wrench. Strike the connector directly.

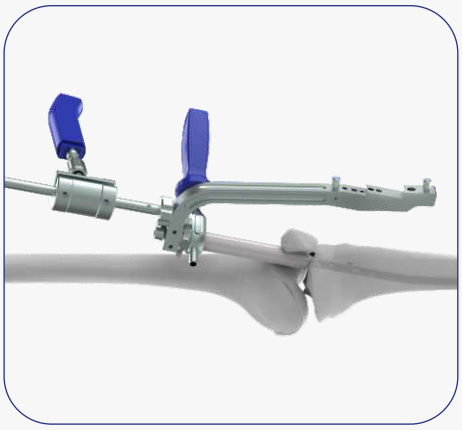

Optionally, the hammer guide can be threaded into the connector and the hammer can be used as a slide hammer. The hammer guide helps to assure the driving cap is struck optimally. Loosen the nut from the threads located below the hammer head and secure onto the threads located above the handle.

4. Check distal nail position

Check final nail position under image intensifier control in AP and lateral views.

Remove the reaming rod.

3. Check proximal nail position

Attach the aiming arm and insert a 3.2 mm guide wire through the hole as shown in the illustration.

The tip of the guide wire indicates the exact proximal position of the tibial nail.

Remove the driving cap.


Remove the aiming arm, unless proximal locking is the next step.

- Check proximal nail position under image intensifier control in the lateral view.

Note:

The distance between the markings on the insertion handle is 5 mm and corresponds to the extensions of the end caps. This feature can be used for overinsertion of the nail or for correcting the nail location within the medullary canal.

If primary compression or secondary dynamization is planned, it is recommended to overinsert the nail by more than 7 mm, which corresponds to the maximum distance between the positions in static and dynamic modes.

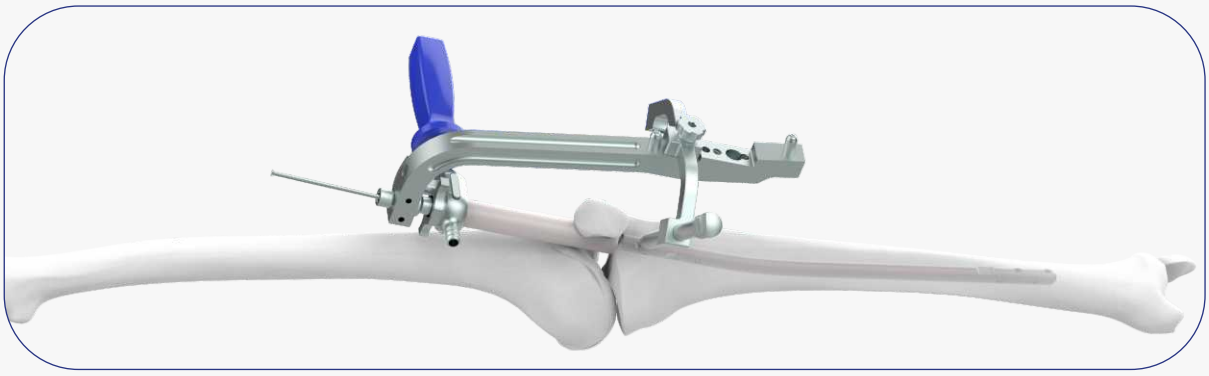

4. Check distal nail position

Check final nail position under image intensifier control in AP and lateral views.

Remove the reaming rod.

1. Determine instrumentation

Use the appropriate locking screws and drill bit for the nail diameter selected.

Locking of the tibial nail is usually performed from the medial side. The knee must be in extension during nail locking. This position helps counteract the forces exerted by the quadriceps muscle that would tend to deform the proximal fragment and also facilitates rotational control of the tibial axis before locking.






2. Align image

- Check the reduction, correct alignment of the fragments, and leg length before locking the nail.

- Align the C-arm with the hole in the nail closest to the fracture until a perfect circle is visible in the center of the screen. (Distal ML hole shown in illustration).


3. Determine incision point

Mount the Distal Aiming Device **(7-112-43)** over the insertion handle and secure it with Bolt for Distal Targeting Device **(7-112-13)**.
Place a guide wire on the skin over the centre of the hole to mark the incision point and make a stab incision. Position the nail with the help of Positioning rod **(7-112-10)** . Mount and secure the Stabilizing device **(7-112-11)** over the Distal targeting arm to secure and lock the nail in-position.

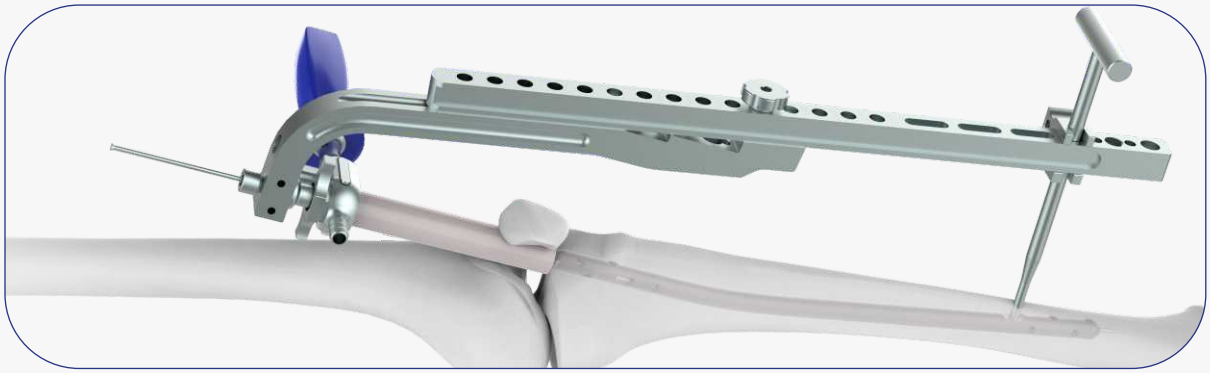


4. Drill

- Using the radiolucent drive under image intensifier. Mount the distal aiming arm **(7-112-12)** over the mounted distal aiming device **(7-112-43)** and secure it with bolt for distal aiming device **(7-112-45)**.
- In place the protection sleeve **(7-112-49)** into the guide of the distal aiming arm (7-112-12). Insert the drill sleeve **(7-112-51)** and drill bit **(7-112-52)** into the protection sleeve and drill drill through both cortices. The drill bit should almost completely fill the circle of the locking hole.

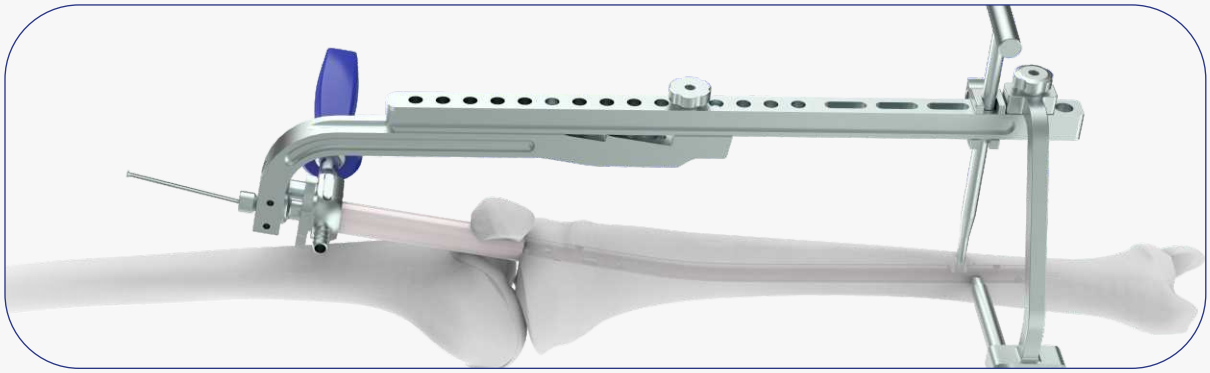


5. Determine locking screw length


Stop drilling immediately after both cortices and disassemble the drill bit from the radiolucent drive.
Under image intensifier control, ensure the correct position of the drill bit beyond the far cortex.
Place the Depth Gauge measuring **(7-112-55)** onto the drill bit. Read the graduation of the measuring device at the end of the drill bit. This corresponds to the appropriate locking screw length.

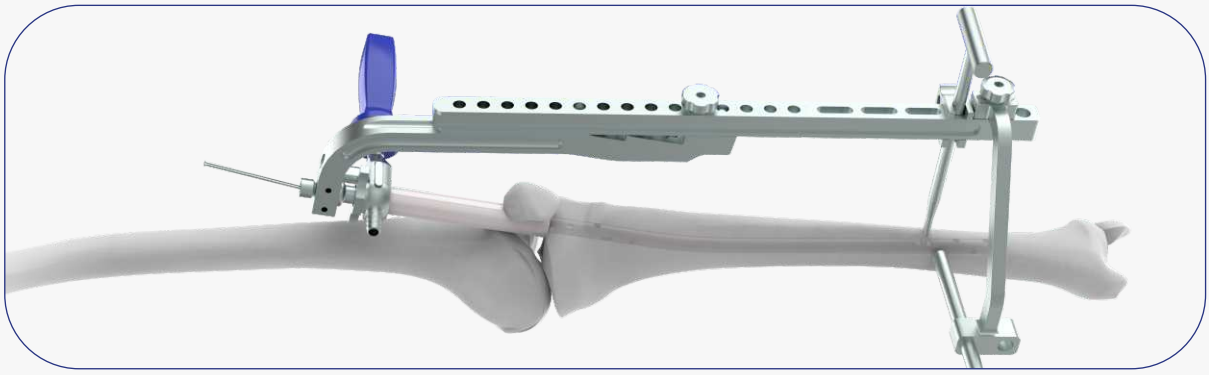


Measure the locking screw length using the depth gauge for locking screws. Ensure the outer sleeve is in contact with the bone and the hook grasps the far cortex.

Read the locking screw length directly from the depth gauge at the back of the outer sleeve.

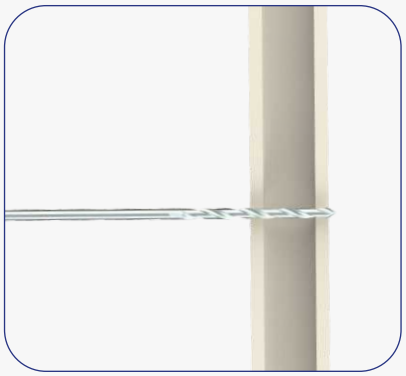

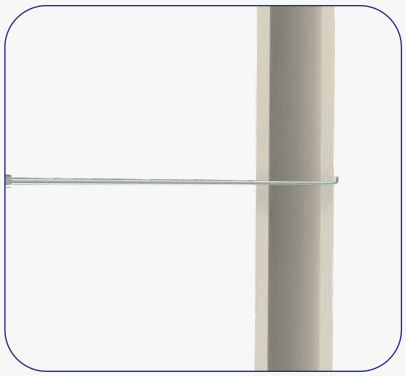

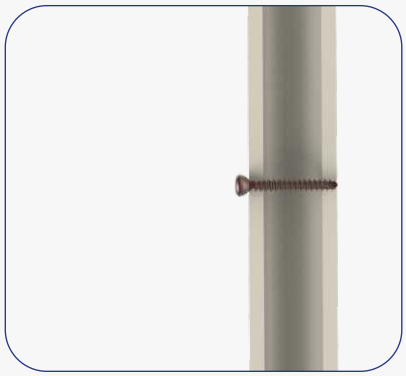


Insert Locking Screw


Insert the appropriate length locking screw using the Screwdriver with T-Handle **(7-112-56)** Screwdriver and the holding sleeve with locking device, if needed.


Verify locking screw length under image intensifier control. If needed, a second locking screw may be inserted using the same technique.


Note:

If compression is desired, the backstroke technique with the hammer guide attached to the connector and insertion handle, light reverse hammer blows may be used to compress the fracture; monitor reduction radiographically. If the nail is overinserted, secure the hammer guide to the driving cap and use the slide hammer. Do not strike directly on the bottom of the insertion handle as this will damage the handle. If using the backstroke technique, distal locking must be performed prior to proximal locking to prevent loss of reduction. Verify the nail has been inserted to the appropriate depth. can be used after insertion of the second distal locking screw. Alternatively, the compression device can be used (refer to section Insert compression device).

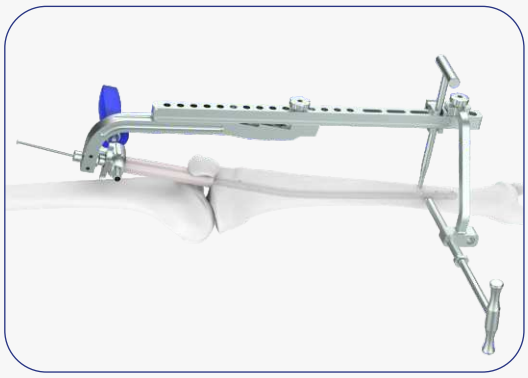

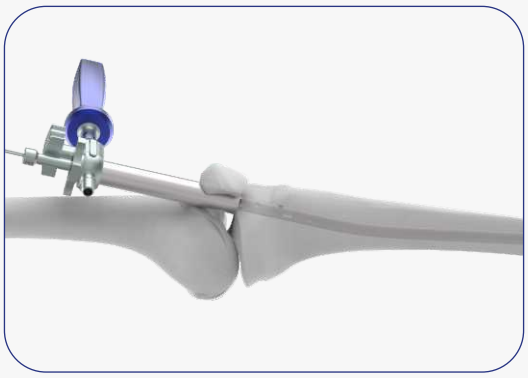

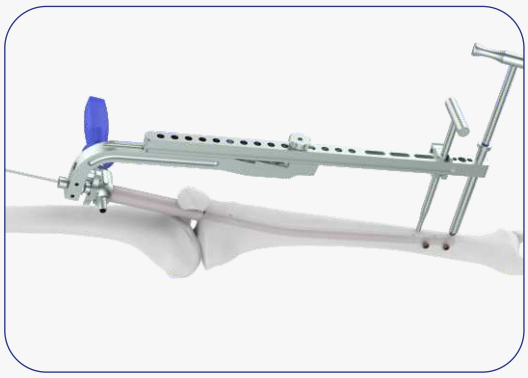

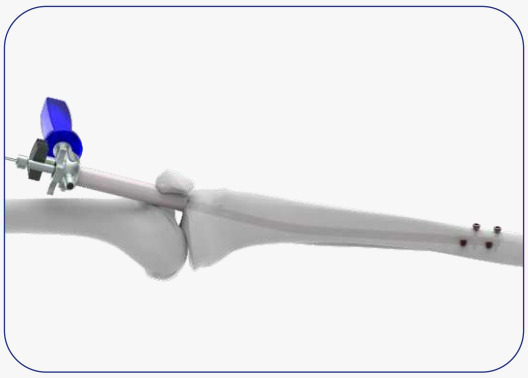

Repeat & follow the steps like drilling, measuring depth as followed in medial to lateral distal locking.

1. Mount aiming arm


Confirm that the nail is securely connected to the insertion handle Mount the Proximal Aiming Device **(7-112-07)** for Ø4.4mm Locking Bolt & secure with Bolt for Proximal Aiming Device **(7-112-08)** to the insertion handle.

Note: Do not exert forces on the aiming arm, protection sleeve, drill sleeves and drill bits. These forces may prevent accurate targeting through the proximal locking holes and damage the drill bits.

2. Insert trocar assembly

Insert the three-part trocar assembly Protection Drill Sleeve 10/8mm **(7-112-49)**, corresponding drill sleeve and Trocar Ø8mm **(7-112-50)** through the desired ML hole in the aiming arm, make a stab incision and insert the trocar to the bone. Remove the trocar.


3. Drill and determine locking screw length

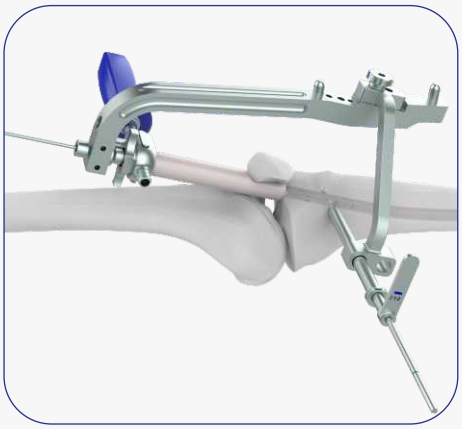

Ensure that the Drill Sleeve 8/4mm for Ø4mm Drill Bit **(7-112-51)** is pressed firmly to the near cortex. Using the corresponding Drill Bit Plain Shank/Jacob Chuck End **(7-112-52)**, drill through both cortices until the tip of the drill bit penetrates the far cortex.

Confirm drill bit position.

Ensure that the drill sleeve is pressed firmly to the near cortex and read the measurement from the calibrated drill bit at the back of the drill sleeve. This measurement corresponds to the appropriate length locking screw. Remove the drill bit and the drill sleeve.

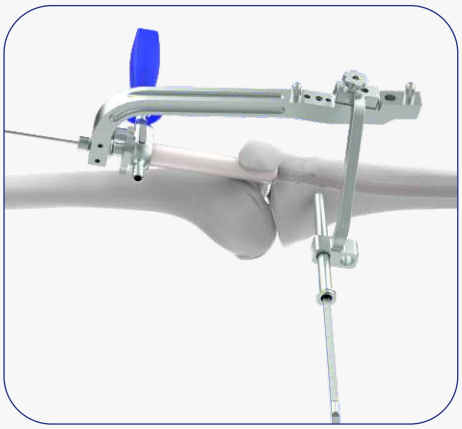


After drilling both cortices, remove the drill bit and the drill sleeve.

Insert the Depth Gauge measuring up-to 90mm **(520-041)** into the protection sleeve. Make sure that the hook grasps the far cortex and that the protection sleeve is on the bone.

Read the measurement from the back of the protection sleeve, which indicates the appropriate length locking screw.

4. Insert locking screw

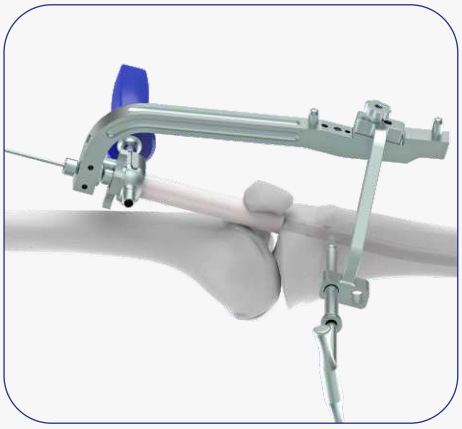

Insert the appropriate length locking screw through the protection sleeve using the Screwdriver with T-Handle, Hex 3.5mm **(7-112-56)** screwdriver. Verify locking screw length under image intensifier control. The tip of the locking screw should not project more than 1–2 mm beyond the far cortex.

Repeat the steps 3 to 5 for the second proximal ML locking screw.

Note: Additional cancellous bone locking screw can be added for proximal fractures and highly unstable fractures.

Proximal Locking - Compression Locking Mode (Optional)

1. Compression locking mode

If the fracture gap needs compression after nail insertion, it can be accomplished without removing the insertion instruments.

The Expert Tibial Nail allows a maximum compression of 7 mm. If more compression of the fracture gap is needed, the conventional backstroke technique.



Distal locking is required prior to compression locking

Insert one proximal locking screw in the dynamic locking hole (DYNAM). For details on inserting this locking screw, refer to section Diaphyseal and Distal Segment Fractures.


2. Insert compression device

If the fracture gap needs compression after nail insertion, it can be accomplished without removing the insertion instruments.

The Expert Tibial Nail allows a maximum compression of 7 mm. If more compression of the fracture gap is needed, the conventional backstroke technique.

Note:

Backstroke technique: with the hammer guide attached to the connector and insertion handle, light reverse hammer blows may be used to compress the fracture; monitor reduction radiographically. If the nail is overinserted, secure the hammer guide to the driving cap and use the slide hammer. Do not strike directly on the bottom of the insertion handle as this will damage the handle. If using the backstroke technique, distal locking must be performed prior to proximal locking to prevent loss of reduction. Verify the nail has been inserted to the appropriate depth.

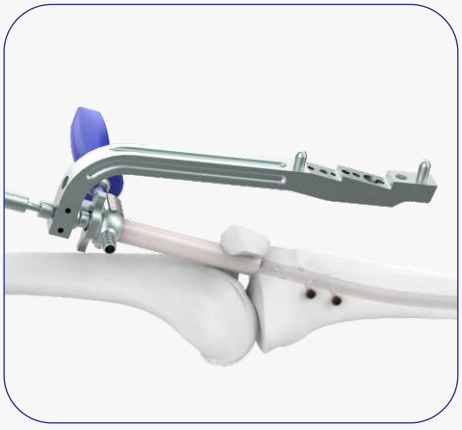

Distal locking is required prior to compression locking.

Insert the compression device **(7-112-16)** into the nail through the insertion handle and compress the screw from top to bottom in the nail slot. Insert one proximal locking screw in the dynamic locking hole (DYNAM). For details on inserting this locking screw, refer to section Diaphyseal and Distal Segment Fractures.

3. Monitor fracture

Control the fracture gap before, during, and after the com pression procedure.




4. Insert static locking screw

Insert second proximal locking screw in the most distal hole of the proximal locking options (Static 1). Refer to section Diaphyseal and Distal Segment Fractures


Remove the compression device.

Additional oblique cancellous bone locking screw can be inserted if required. Refer to section Proximal Segment Fractures.

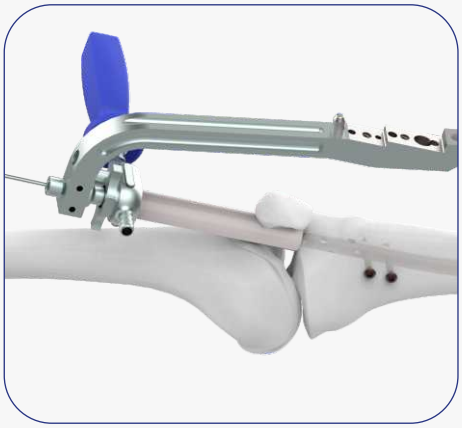

1. Oblique proximal locking

Proximal locking is performed with the knee in extension when using the suprapatellar technique. This neutralizes the deforming forces on proximal fragments caused by the quadriceps mechanism and relieves the pressure on the soft tissue usually associated with tibial nail insertion instruments. This position also facilitates assessment of rotational alignment prior to locking.

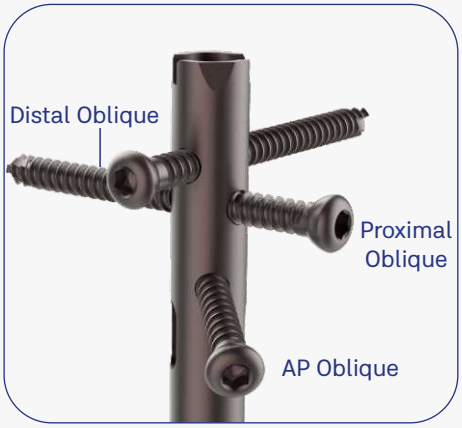


Note: When locking with the leg in full extension, it is recommended to use the insertion handle for Expert Tibial Nail and cannulated connecting screw to prevent impingement on the patella. These devices are not compatible with the compression device.

The aiming arm can target all three proximal oblique locking options:

1. The oblique locking option (PROXIMAL OBLIQUE) corresponds to the most proximal locking position. Inserting a tibial nail end cap with this locking screw will create a fixed-angle construct.
2. The oblique locking option (DISTAL OBLIQUE) corresponds to the second proximal locking position.
3. The oblique locking option in anteroposterior direction (A/P) corresponds to the third proximal locking position.


2. Mount aiming arm

Confirm that the nail is securely connected to the insertion handle using the screwdriver. Mount the Proximal Aiming Device for Ø4.8mm Locking Bolt **(7-112-09)** to the insertion handle & secure it with the Bolt for Proximal Aiming Device **(7-112-08)** as shown in the illustration.

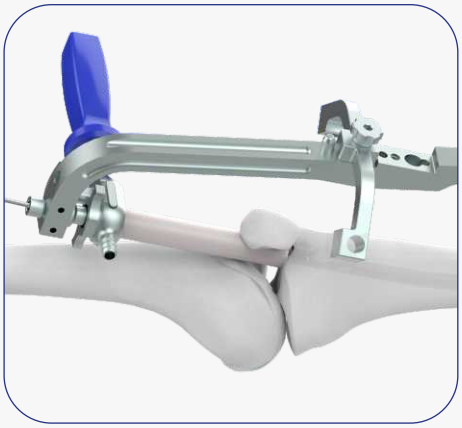

Note: Do not exert forces on the aiming arm, protection sleeve, drill sleeves and drill bits. These forces may prevent accurate targeting through the proximal locking holes and damage the drill bits.

3. Insert trocar assembly

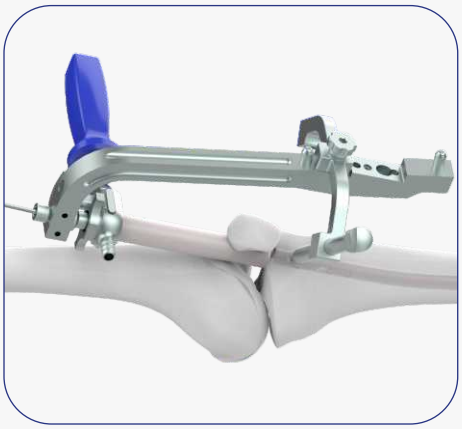


Insert the three-part trocar assembly (Protection Sleeve 11/8.6mm **(7-112-57)**, Drill Sleeve 8.5/3.2mm for Ø3.2mm **(7-112-58)**, Trocar Ø3.2mm **(7-112-59)** through the desired hole for oblique locking options in the aiming arm, make a stab incision and insert the trocar to the bone. Remove the trocar.

4. Drill and determine dual core locking screw length

Ensure that the drill sleeve is pressed firmly to the near cortex.

Insert the calibrated Drill Bit Plain Shank/Jacob Chuck End Ø3.2mm **(7-112-60)** and start drilling the near cortex.

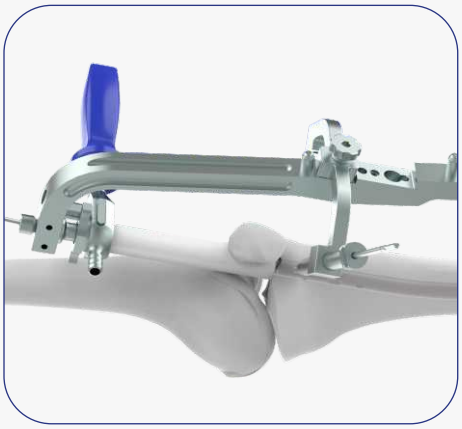

Precaution: Stop drilling immediately after penetrating the near cortex.


DO NOT penetrate the far cortex.

Monitor the position of the drill bit with the image Intensifier. This can be done by orienting the image intensifier perpendicular to the drill bit.

Drill to the desired depth. A long dual core locking screw will achieve better bone purchase than a shorter dual core locking screw.

Precaution: Do not perforate the far cortex with the drill bit. Do not damage the tibial plateau.

- Confirm drill bit position after drilling.

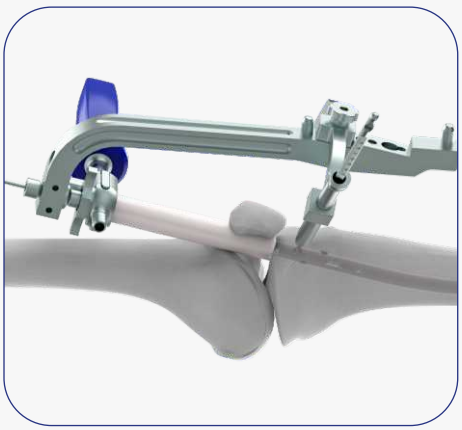

Ensure that the drill sleeve is pressed firmly to the bone and read the measurement from the Depth Gauge measuring **(520-041)** at the back of the drill sleeve.


This measurement indicates the appropriate length of the dual core locking screw.

Remove the drill bit and the drill sleeve.

Precaution: To avoid perforation of the far cortex with the dual core locking screw, a dual core locking screw 5 mm shorter than the measured length is recommended.

5. Insert cancellous bone locking screw

Insert the appropriate 4.8 mm dual core locking screw through the protection sleeve, using the Screwdriver with T-Handle, Hex 3.5mm **(7-112-56)**.

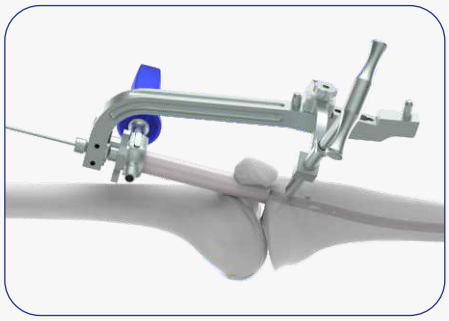


Do not overtighten.


- Verify locking screw length under image intensifier control.

Repeat this procedure for the second dual core locking screw.

If required, repeat the steps described above for the third proximal dual core locking screw in the AP direction.

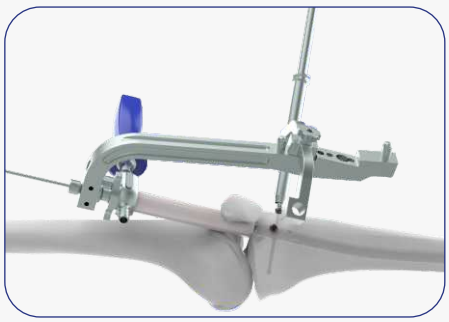

The position of the dual core locking screw should be controlled with the image intensifier to ensure a correct position of the AP dual core locking screw.

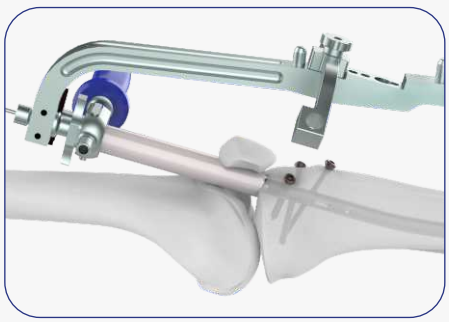

End Cap Insertion


End Cap insertion: In order to prevent tissue growth inside the nail, end cap insertion is required. The insertion handle is detached from the nail and using the Screwdriver with T-Handle, Hex 3.5mm **(7-112-56)** , advance the end cap into the nail.

All titanium end caps for Expert Tibial Nails are available in extension lengths of 0 mm, 5 mm, 10 mm, and 15 mm. They prevent bone ingrowth into the nail and they extend the nail height if it is over inserted. The gold end caps lock the proximal oblique screw providing a stable fixed-angle construct.

Remove the connecting screw. The insertion handle can remain in place to help align the end cap to the top of the nail. The end cap fits through the barrel of the insertion handle.

Alternatively, remove the connecting screw and insertion handle. Reinsert the inner protection sleeve to open the cannula through the outer protection sleeve.



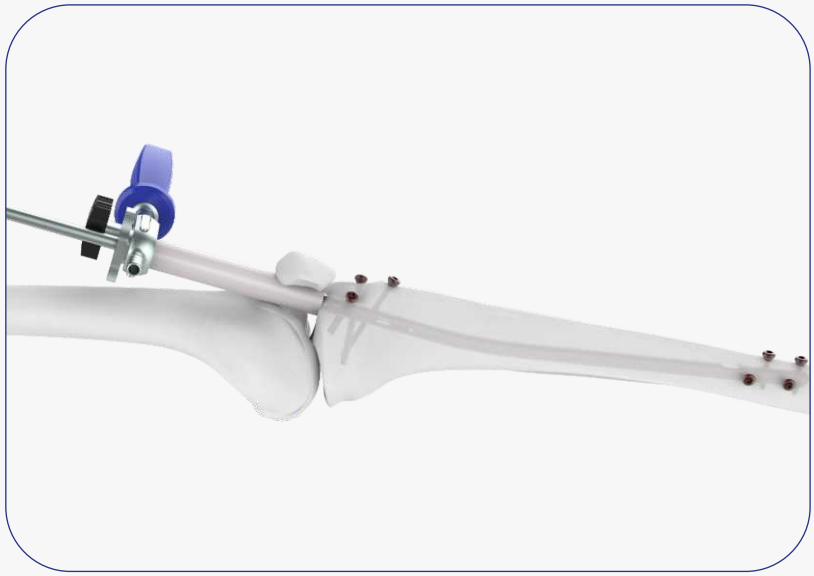

Alternative instruments

The end caps are cannulated and can be used over a guide wire with the cannulated screwdriver.



Engage the end cap with the cannulated screwdriver, inter-lock. To prevent cross threading, align the end cap with the nail axis and turn the end cap counterclockwise, until the thread of the end cap aligns with that of the nail.

Turn the end cap clockwise to thread the end cap into the nail. Remove the guide wire and screwdriver.

Implant Removal

In case of implant removal firstly remove the end cap with the help of 3.5mm Hex screwdriver. Proceed by removing both Ø4.4mm and Ø4.8mm Locking Bolt from the bone using 3.5mm Hex screwdriver. Attach the connecting shaft **(520-019)** to the open end of nail from where the end cap is removed.



On top of connecting shaft attach the Hammer guide shaft **(520-022)** followed by screwing the nut for hammer guide shaft **(520-023)** on top of hammer guide shaft. Unlock the nut on the sliding hammer **(520-024)** for its free movement during nail removal. Now, slide the Sliding Hammer into the hammer guide shaft. Strike the hammer in upward direction to remove the nail from the bone.



Note: It is highly recommended not to remove all the locking bolt as it may cause the nail rotation during attachment of the connecting shaft to the nail. Remove the remaining Locking bolt after the connecting shaft and the hammer guide shaft has been attached.

Expert Tibia Nail

NON STERILE

Stainless Steel

	Code	Dia x Length
Ø8mm	520-08-255	Ø8mm x 255mm
	520-08-270	Ø8mm x 270mm
	520-08-285	Ø8mm x 285mm
	520-08-300	Ø8mm x 300mm
	520-08-315	Ø8mm x 315mm
	520-08-330	Ø8mm x 330mm
	520-08-345	Ø8mm x 345mm
	520-08-360	Ø8mm x 360mm
	520-08-375	Ø8mm x 375mm
Ø9mm	520-09-255	Ø9mm x 255mm
	520-09-270	Ø9mm x 270mm
	520-09-285	Ø9mm x 285mm
	520-09-300	Ø9mm x 300mm
	520-09-315	Ø9mm x 315mm
	520-09-330	Ø9mm x 330mm
	520-09-345	Ø9mm x 345mm
	520-09-360	Ø9mm x 360mm
	520-09-375	Ø9mm x 375mm
Ø10mm	520-10-255	Ø10mm x 255mm
	520-10-270	Ø10mm x 270mm
	520-10-285	Ø10mm x 285mm
	520-10-300	Ø10mm x 300mm
	520-10-315	Ø10mm x 315mm
	520-10-330	Ø10mm x 330mm
	520-10-345	Ø10mm x 345mm
	520-10-360	Ø10mm x 360mm
	520-10-375	Ø10mm x 375mm
Ø11mm	520-11-255	Ø11mm x 255mm
	520-11-270	Ø11mm x 270mm
	520-11-285	Ø11mm x 285mm
	520-11-300	Ø11mm x 300mm
	520-11-315	Ø11mm x 315mm
	520-11-330	Ø11mm x 330mm
	520-11-345	Ø11mm x 345mm
	520-11-360	Ø11mm x 360mm
	520-11-375	Ø11mm x 375mm
Ø12mm	520-12-255	Ø12mm x 255mm
	520-12-270	Ø12mm x 270mm
	520-12-285	Ø12mm x 285mm
	520-12-300	Ø12mm x 300mm
	520-12-315	Ø12mm x 315mm
	520-12-330	Ø12mm x 330mm
	520-12-345	Ø12mm x 345mm
	520-12-360	Ø12mm x 360mm
	520-12-375	Ø12mm x 375mm



Titanium

	Code	Dia x Length
Ø8mm	TI-520-08-255	Ø8mm x 255mm
	TI-520-08-270	Ø8mm x 270mm
	TI-520-08-285	Ø8mm x 285mm
	TI-520-08-300	Ø8mm x 300mm
	TI-520-08-315	Ø8mm x 315mm
	TI-520-08-330	Ø8mm x 330mm
	TI-520-08-345	Ø8mm x 345mm
	TI-520-08-360	Ø8mm x 360mm
	TI-520-08-375	Ø8mm x 375mm
Ø9mm	TI-520-09-255	Ø9mm x 255mm
	TI-520-09-270	Ø9mm x 270mm
	TI-520-09-285	Ø9mm x 285mm
	TI-520-09-300	Ø9mm x 300mm
	TI-520-09-315	Ø9mm x 315mm
	TI-520-09-330	Ø9mm x 330mm
	TI-520-09-345	Ø9mm x 345mm
	TI-520-09-360	Ø9mm x 360mm
	TI-520-09-375	Ø9mm x 375mm
Ø10mm	TI-520-10-255	Ø10mm x 255mm
	TI-520-10-270	Ø10mm x 270mm
	TI-520-10-285	Ø10mm x 285mm
	TI-520-10-300	Ø10mm x 300mm
	TI-520-10-315	Ø10mm x 315mm
	TI-520-10-330	Ø10mm x 330mm
	TI-520-10-345	Ø10mm x 345mm
	TI-520-10-360	Ø10mm x 360mm
	TI-520-10-375	Ø10mm x 375mm
Ø11mm	TI-520-11-255	Ø11mm x 255mm
	TI-520-11-270	Ø11mm x 270mm
	TI-520-11-285	Ø11mm x 285mm
	TI-520-11-300	Ø11mm x 300mm
	TI-520-11-315	Ø11mm x 315mm
	TI-520-11-330	Ø11mm x 330mm
	TI-520-11-345	Ø11mm x 345mm
	TI-520-11-360	Ø11mm x 360mm
	TI-520-11-375	Ø11mm x 375mm
Ø12mm	TI-520-12-255	Ø12mm x 255mm
	TI-520-12-270	Ø12mm x 270mm
	TI-520-12-285	Ø12mm x 285mm
	TI-520-12-300	Ø12mm x 300mm
	TI-520-12-315	Ø12mm x 315mm
	TI-520-12-330	Ø12mm x 330mm
	TI-520-12-345	Ø12mm x 345mm
	TI-520-12-360	Ø12mm x 360mm
	TI-520-12-375	Ø12mm x 375mm



Expert Tibia Nail

STERILE

Stainless Steel

	Code	Dia x Length
Ø8mm	520-08-255-S	Ø8mm x 255mm
	520-08-270-S	Ø8mm x 270mm
	520-08-285-S	Ø8mm x 285mm
	520-08-300-S	Ø8mm x 300mm
	520-08-315-S	Ø8mm x 315mm
	520-08-330-S	Ø8mm x 330mm
	520-08-345-S	Ø8mm x 345mm
	520-08-360-S	Ø8mm x 360mm
	520-08-375-S	Ø8mm x 375mm
Ø9mm	520-09-255-S	Ø9mm x 255mm
	520-09-270-S	Ø9mm x 270mm
	520-09-285-S	Ø9mm x 285mm
	520-09-300-S	Ø9mm x 300mm
	520-09-315-S	Ø9mm x 315mm
	520-09-330-S	Ø9mm x 330mm
	520-09-345-S	Ø9mm x 345mm
	520-09-360-S	Ø9mm x 360mm
	520-09-375-S	Ø9mm x 375mm
Ø10mm	520-10-255-S	Ø10mm x 255mm
	520-10-270-S	Ø10mm x 270mm
	520-10-285-S	Ø10mm x 285mm
	520-10-300-S	Ø10mm x 300mm
	520-10-315-S	Ø10mm x 315mm
	520-10-330-S	Ø10mm x 330mm
	520-10-345-S	Ø10mm x 345mm
	520-10-360-S	Ø10mm x 360mm
	520-10-375-S	Ø10mm x 375mm
Ø11mm	520-11-255-S	Ø11mm x 255mm
	520-11-270-S	Ø11mm x 270mm
	520-11-285-S	Ø11mm x 285mm
	520-11-300-S	Ø11mm x 300mm
	520-11-315-S	Ø11mm x 315mm
	520-11-330-S	Ø11mm x 330mm
	520-11-345-S	Ø11mm x 345mm
	520-11-360-S	Ø11mm x 360mm
	520-11-375-S	Ø11mm x 375mm
Ø12mm	520-12-255-S	Ø12mm x 255mm
	520-12-270-S	Ø12mm x 270mm
	520-12-285-S	Ø12mm x 285mm
	520-12-300-S	Ø12mm x 300mm
	520-12-315-S	Ø12mm x 315mm
	520-12-330-S	Ø12mm x 330mm
	520-12-345-S	Ø12mm x 345mm
	520-12-360-S	Ø12mm x 360mm
	520-12-375-S	Ø12mm x 375mm



Titanium

	Code	Dia x Length
Ø8mm	TI-520-08-255-S	Ø8mm x 255mm
	TI-520-08-270-S	Ø8mm x 270mm
	TI-520-08-285-S	Ø8mm x 285mm
	TI-520-08-300-S	Ø8mm x 300mm
	TI-520-08-315-S	Ø8mm x 315mm
	TI-520-08-330-S	Ø8mm x 330mm
	TI-520-08-345-S	Ø8mm x 345mm
	TI-520-08-360-S	Ø8mm x 360mm
	TI-520-08-375-S	Ø8mm x 375mm
Ø9mm	TI-520-09-255-S	Ø9mm x 255mm
	TI-520-09-270-S	Ø9mm x 270mm
	TI-520-09-285-S	Ø9mm x 285mm
	TI-520-09-300-S	Ø9mm x 300mm
	TI-520-09-315-S	Ø9mm x 315mm
	TI-520-09-330-S	Ø9mm x 330mm
	TI-520-09-345-S	Ø9mm x 345mm
	TI-520-09-360-S	Ø9mm x 360mm
	TI-520-09-375-S	Ø9mm x 375mm
Ø10mm	TI-520-10-255-S	Ø10mm x 255mm
	TI-520-10-270-S	Ø10mm x 270mm
	TI-520-10-285-S	Ø10mm x 285mm
	TI-520-10-300-S	Ø10mm x 300mm
	TI-520-10-315-S	Ø10mm x 315mm
	TI-520-10-330-S	Ø10mm x 330mm
	TI-520-10-345-S	Ø10mm x 345mm
	TI-520-10-360-S	Ø10mm x 360mm
	TI-520-10-375-S	Ø10mm x 375mm
Ø11mm	TI-520-11-255-S	Ø11mm x 255mm
	TI-520-11-270-S	Ø11mm x 270mm
	TI-520-11-285-S	Ø11mm x 285mm
	TI-520-11-300-S	Ø11mm x 300mm
	TI-520-11-315-S	Ø11mm x 315mm
	TI-520-11-330-S	Ø11mm x 330mm
	TI-520-11-345-S	Ø11mm x 345mm
	TI-520-11-360-S	Ø11mm x 360mm
	TI-520-11-375-S	Ø11mm x 375mm
Ø12mm	TI-520-12-255-S	Ø12mm x 255mm
	TI-520-12-270-S	Ø12mm x 270mm
	TI-520-12-285-S	Ø12mm x 285mm
	TI-520-12-300-S	Ø12mm x 300mm
	TI-520-12-315-S	Ø12mm x 315mm
	TI-520-12-330-S	Ø12mm x 330mm
	TI-520-12-345-S	Ø12mm x 345mm
	TI-520-12-360-S	Ø12mm x 360mm
	TI-520-12-375-S	Ø12mm x 375mm



End Cap For Expert Tibia Nail



NON STERILE

Stainless Steel	Titanium	Length
520-001	TI-520-001	0mm
520-001-05	TI-520-001-05	5mm
520-001-10	TI-520-001-10	10mm
520-001-15	TI-520-001-15	15mm

STERILE

Stainless Steel	Titanium	Length
520-001-S	TI-520-001-S	0mm
520-001-05-S	TI-520-001-05-S	5mm
520-001-10-S	TI-520-001-10-S	10mm
520-001-15-S	TI-520-001-15-S	15mm

Ø4.8mm Locking Bolt, Self-Tapping, For Expert Tibia Nail



NON STERILE

Stainless Steel	Titanium	Length
520-002-25	TI-520-002-25	25mm
520-002-30	TI-520-002-30	30mm
520-002-35	TI-520-002-35	35mm
520-002-40	TI-520-002-40	40mm
520-002-45	TI-520-002-45	45mm
520-002-50	TI-520-002-50	50mm
520-002-55	TI-520-002-55	55mm
520-002-60	TI-520-002-60	60mm
520-002-65	TI-520-002-65	65mm
520-002-70	TI-520-002-70	70mm
520-002-75	TI-520-002-75	75mm
520-002-80	TI-520-002-80	80mm
520-002-85	TI-520-002-85	85mm
520-002-90	TI-520-002-90	90mm

STERILE

Stainless Steel	Titanium	Length
520-002-25-S	TI-520-002-25-S	25mm
520-002-30-S	TI-520-002-30-S	30mm
520-002-35-S	TI-520-002-35-S	35mm
520-002-40-S	TI-520-002-40-S	40mm
520-002-45-S	TI-520-002-45-S	45mm
520-002-50-S	TI-520-002-50-S	50mm
520-002-55-S	TI-520-002-55-S	55mm
520-002-60-S	TI-520-002-60-S	60mm
520-002-65-S	TI-520-002-65-S	65mm
520-002-70-S	TI-520-002-70-S	70mm
520-002-75-S	TI-520-002-75-S	75mm
520-002-80-S	TI-520-002-80-S	80mm
520-002-85-S	TI-520-002-85-S	85mm
520-002-90-S	TI-520-002-90-S	90mm

Ø4.4mm Locking Bolt, Self-Tapping, For Expert Tibia Nail,

NON STERILE

Stainless Steel	Titanium	Length
520-058-24	TI-520-058-24	24mm
520-058-26	TI-520-058-26	26mm
520-058-28	TI-520-058-28	28mm
520-058-30	TI-520-058-30	30mm
520-058-32	TI-520-058-32	32mm
520-058-34	TI-520-058-34	34mm
520-058-36	TI-520-058-36	36mm
520-058-38	TI-520-058-38	38mm
520-058-40	TI-520-058-40	40mm
520-058-42	TI-520-058-42	42mm
520-058-44	TI-520-058-44	44mm
520-058-46	TI-520-058-46	46mm
520-058-48	TI-520-058-48	48mm
520-058-50	TI-520-058-50	50mm
520-058-52	TI-520-058-52	52mm
520-058-54	TI-520-058-54	54mm
520-058-56	TI-520-058-56	56mm
520-058-58	TI-520-058-58	58mm
520-058-60	TI-520-058-60	60mm
520-058-62	TI-520-058-62	62mm
520-058-64	TI-520-058-64	64mm
520-058-66	TI-520-058-66	66mm
520-058-68	TI-520-058-68	68mm
520-058-70	TI-520-058-70	70mm
520-058-72	TI-520-058-72	72mm
520-058-74	TI-520-058-74	74mm
520-058-76	TI-520-058-76	76mm
520-058-78	TI-520-058-78	78mm
520-058-80	TI-520-058-80	80mm
520-058-82	TI-520-058-82	82mm
520-058-84	TI-520-058-84	84mm
520-058-86	TI-520-058-86	86mm
520-058-88	TI-520-058-88	88mm



STERILE

Stainless Steel	Titanium	Length
520-058-24-S	TI-520-058-24-S	24mm
520-058-26-S	TI-520-058-26-S	26mm
520-058-28-S	TI-520-058-28-S	28mm
520-058-30-S	TI-520-058-30-S	30mm
520-058-32-S	TI-520-058-32-S	32mm
520-058-34-S	TI-520-058-34-S	34mm
520-058-36-S	TI-520-058-36-S	36mm
520-058-38-S	TI-520-058-38-S	38mm
520-058-40-S	TI-520-058-40-S	40mm
520-058-42-S	TI-520-058-42-S	42mm
520-058-44-S	TI-520-058-44-S	44mm
520-058-46-S	TI-520-058-46-S	46mm
520-058-48-S	TI-520-058-48-S	48mm
520-058-50-S	TI-520-058-50-S	50mm
520-058-52-S	TI-520-058-52-S	52mm
520-058-54-S	TI-520-058-54-S	54mm
520-058-56-S	TI-520-058-56-S	56mm
520-058-58-S	TI-520-058-58-S	58mm
520-058-60-S	TI-520-058-60-S	60mm
520-058-62-S	TI-520-058-62-S	62mm
520-058-64-S	TI-520-058-64-S	64mm
520-058-66-S	TI-520-058-66-S	66mm
520-058-68-S	TI-520-058-68-S	68mm
520-058-70-S	TI-520-058-70-S	70mm
520-058-72-S	TI-520-058-72-S	72mm
520-058-74-S	TI-520-058-74-S	74mm
520-058-76-S	TI-520-058-76-S	76mm
520-058-78-S	TI-520-058-78-S	78mm
520-058-80-S	TI-520-058-80-S	80mm
520-058-82-S	TI-520-058-82-S	82mm
520-058-84-S	TI-520-058-84-S	84mm
520-058-86-S	TI-520-058-86-S	86mm
520-058-88-S	TI-520-058-88-S	88mm

Optional

Ø4.4mm Locking Bolt, Self-Tapping, For Expert Tibia Nail-Old Design

NON STERILE

Stainless Steel	Titanium	Length
520-058-24-OD	TI-520-058-24-OD	24mm
520-058-26-OD	TI-520-058-26-OD	26mm
520-058-28-OD	TI-520-058-28-OD	28mm
520-058-30-OD	TI-520-058-30-OD	30mm
520-058-32-OD	TI-520-058-32-OD	32mm
520-058-34-OD	TI-520-058-34-OD	34mm
520-058-36-OD	TI-520-058-36-OD	36mm
520-058-38-OD	TI-520-058-38-OD	38mm
520-058-40-OD	TI-520-058-40-OD	40mm
520-058-42-OD	TI-520-058-42-OD	42mm
520-058-44-OD	TI-520-058-44-OD	44mm
520-058-46-OD	TI-520-058-46-OD	46mm
520-058-48-OD	TI-520-058-48-OD	48mm
520-058-50-OD	TI-520-058-50-OD	50mm
520-058-52-OD	TI-520-058-52-OD	52mm
520-058-54-OD	TI-520-058-54-OD	54mm
520-058-56-OD	TI-520-058-56-OD	56mm
520-058-58-OD	TI-520-058-58-OD	58mm
520-058-60-OD	TI-520-058-60-OD	60mm
520-058-62-OD	TI-520-058-62-OD	62mm
520-058-64-OD	TI-520-058-64-OD	64mm
520-058-66-OD	TI-520-058-66-OD	66mm
520-058-68-OD	TI-520-058-68-OD	68mm
520-058-70-OD	TI-520-058-70-OD	70mm
520-058-72-OD	TI-520-058-72-OD	72mm
520-058-74-OD	TI-520-058-74-OD	74mm
520-058-76-OD	TI-520-058-76-OD	76mm
520-058-78-OD	TI-520-058-78-OD	78mm
520-058-80-OD	TI-520-058-80-OD	80mm
520-058-82-OD	TI-520-058-82-OD	82mm
520-058-84-OD	TI-520-058-84-OD	84mm
520-058-86-OD	TI-520-058-86-OD	86mm
520-058-88-OD	TI-520-058-88-OD	88mm



Ø4.8mm Locking Bolt, Self-Tapping, For Expert Tibia Nail-Old Design

NON STERILE

Stainless Steel	Titanium	Length
520-002-25-OD	TI-520-002-25-OD	25mm
520-002-30-OD	TI-520-002-30-OD	30mm
520-002-35-OD	TI-520-002-35-OD	35mm
520-002-40-OD	TI-520-002-40-OD	40mm
520-002-45-OD	TI-520-002-45-OD	45mm
520-002-50-OD	TI-520-002-50-OD	50mm
520-002-55-OD	TI-520-002-55-OD	55mm
520-002-60-OD	TI-520-002-60-OD	60mm
520-002-65-OD	TI-520-002-65-OD	65mm
520-002-70-OD	TI-520-002-70-OD	70mm
520-002-75-OD	TI-520-002-75-OD	75mm
520-002-80-OD	TI-520-002-80-OD	80mm
520-002-85-OD	TI-520-002-85-OD	85mm
520-002-90-OD	TI-520-002-90-OD	90mm




IMPLANT SET

1-013	Implant Box for Expert Tibia Nailing




Tray 1

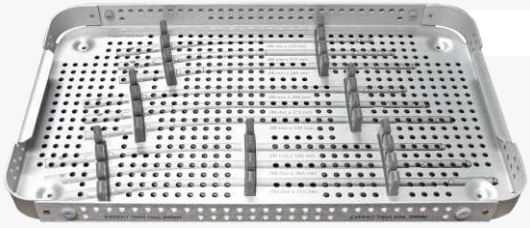

Dia	Length	Qty
Ø8mm	255mm to 375mm	1pcs

Stainless Steel or Titanium Implants
can be placed as per requirement


Tray 2

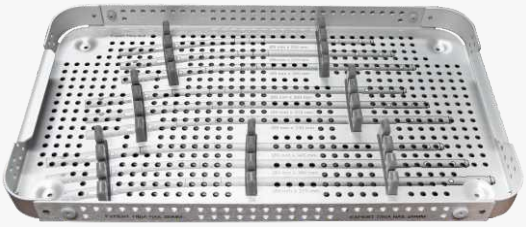

Dia	Length	Qty
Ø9mm	255mm to 375mm	1pcs

Stainless Steel or Titanium Implants
can be placed as per requirement


Tray 3

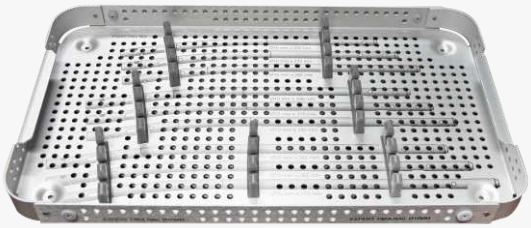

Dia	Length	Qty
Ø10mm	255mm to 375mm	1pcs

Stainless Steel or Titanium Implants
can be placed as per requirement


Tray 4

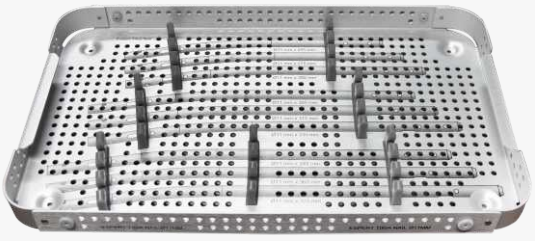

Dia	Length	Qty
Ø11mm	255mm to 375mm	1pcs

Stainless Steel or Titanium Implants
can be placed as per requirement

Tray 5

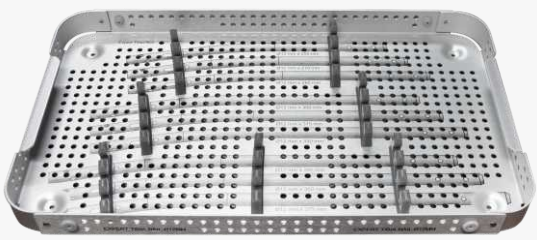

Dia	Length	Qty
Ø12mm	255mm to 375mm	1pcs

Stainless Steel or Titanium Implants
can be placed as per requirement



Ø4.8mm Locking Bolt, Self-Tapping, For Expert Tibia Nail

Dia	Length	Qty
Ø4.8mm	25mm to 90mm	3pcs

Stainless Steel or Titanium Implants can be placed as per requirement

Ø4.4mm Locking Bolt, Self-Tapping, For Expert Tibia Nail

Dia	Length	Qty
Ø4.4mm	24mm to 88mm	6pcs

Stainless Steel or Titanium Implants can be placed as per requirement

End Cap For Expert Tibia Nail

Length	Qty
0mm to 15mm	2pcs

Stainless Steel or Titanium Implants can be placed as per requirement

INSTRUMENT SET

(SUPRAPATELLAR INSERTION)

7-112-01

Insertion Handle for Expert Tibia Nail - Suprapatellar Insertion



7-112-02

Protection Sleeve Handle for Expert Tibia Nail - Suprapatellar Insertion



7-112-03

Outer Protection Sleeve for Expert Tibia Nail - Suprapatellar Insertion



7-112-04

Protection Sleeve 16/14.5mm for Expert Tibia Nail - Suprapatellar Insertion



7-112-05

Trocar Ø14.5mm, PEEK, for Expert Tibia Nail - Suprapatellar Insertion



7-112-06

Centering Sleeve 14.5/3.2mm for Expert Tibia Nail - Suprapatellar Insertion



7-112-07

Proximal Aiming Device for Ø4.4mm Locking Bolt - Expert Tibia Nail (Suprapatellar Insertion)



7-112-08

Bolt for Proximal Aiming Device - Expert Tibia Nail (Suprapatellar Insertion)



7-112-09

Proximal Aiming Device for Ø4.8mm Locking Bolt - Expert Tibia Nail (Suprapatellar Insertion)



7-112-10

Positioning Rod For Expert Tibia Nail - Suprapatellar Insertion



7-112-11

Stabilizing Device for Expert Tibia Nail - Suprapatellar Insertion



7-112-12

Distal Aiming Arm for Expert Tibia Nail - Suprapatellar Insertion



7-112-13 Bolt for Distal Targeting Device, for Expert Tibia Nail - Suprapatellar Insertion



7-112-14 Universal Driver for Nail Holding Bolt - Expert Tibia Nail (Suprapatellar Insertion)



7-112-15 Entry Reamer for Expert Tibia Nail - Suprapatellar Insertion



7-112-16 Compression Device for Expert Tibia Nail - Suprapatellar Insertion



7-112-17 Extraction Screw for Expert Tibia Nail - Suprapatellar Insertion



7-112-18 Connecting Shaft for Expert Tibia Nail - Suprapatellar Insertion



7-112-19

Nail Holding Bolt, Long, for Expert Tibia Nail - Suprapatellar Insertion



7-112-20

Combination Wrench 11mm for Expert Tibia Nail - Suprapatellar Insertion



7-112-21

Sliding Hammer for Expert Tibia Nail - Suprapatellar Insertion



7-112-22

Hammer Guide Shaft for Expert Tibia Nail - Suprapatellar Insertion



7-112-23

Nut for Hammer Guide Shaft - Expert Tibia Nail - Suprapatellar Insertion



7-112-24

Radiographic Ruler for Expert Tibia Nail - Suprapatellar Insertion



520-004

Guide Wire With Threaded Tip Ø3.2mm x Thread Length 10mm x Length 300mm

7-112-25

Entry Cutter for Expert Tibia Nail - Suprapatellar Insertion



7-112-26

Quick Coupling T Handle for Expert Tibia Nail - Suprapatellar Insertion



7-112-27

Cannulated Awl for Expert Tibia Nail - Suprapatellar Insertion




7-112-28

Reduction Device for Expert Tibia Nail - Suprapatellar Insertion




520-013

Guide wire with Ball Tip Ø2.5/3.65mm x Length 1000mm - Nitinol, for Expert Tibia Nail

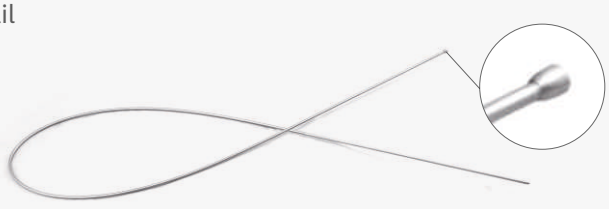

520-058

Guide wire without Ball Tip Ø2.5mm x Length 1000mm - Nitinol, for Expert Tibia Nail

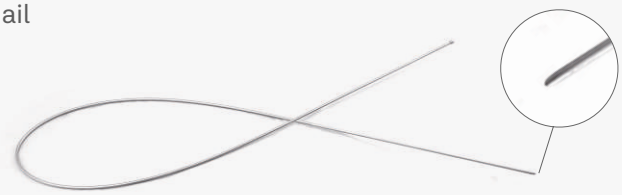

7-112-29

Guide Wire Holder for Expert Tibia Nail - Suprapatellar Insertion



7-112-30

Flexible Reamer Shaft (AO Connection) for Expert Tibia Nail - Suprapatellar Insertion, Length 620mm



Reamer Head

Dia	Code
Ø7.5mm	7-112-31
Ø8mm	7-112-32
Ø8.5mm	7-112-33
Ø9mm	7-112-34
Ø9.5mm	7-112-35
Ø10mm	7-112-36

Dia	Code
Ø10.5mm	7-112-37
Ø11mm	7-112-38
Ø11.5mm	7-112-39
Ø12mm	7-112-40
Ø12.5mm	7-112-41
Ø13mm	7-112-42



7-112-43

Distal Aiming Device for Expert Tibia Nail - Suprapatellar Insertion




7-112-44

Ø5.2mm T-Handle Drill Bit with Flat End for Expert Tibia Nail - Suprapatellar Insertion



7-112-45

Bolt for Distal Aiming Arm - Expert Tibia Nail (Suprapatellar Insertion)



7-112-46

Allen Key, Hex 5mm for Expert Tibia Nail (Suprapatellar Insertion)



7-112-47

Drill Sleeve, Ø5.2mm for Positioning Rod - Expert Tibia Nail (Suprapatellar Insertion)



7-112-48

Drill Bit Plain Shank/ Jacob Chuck End Ø5.2mm x Length 250mm for Expert Tibia Nail (Suprapatellar Insertion)



7-112-49

Protection Drill Sleeve 10/8mm for Expert Tibia Nail (Suprapatellar Insertion)



7-112-50

Trocar Ø8mm for Expert Tibia Nail (Suprapatellar Insertion)



7-112-51

Drill Sleeve 8/4mm for Ø4mm Drill Bit - Expert Tibia Nail (suprapatellar Insertion)



7-112-52

Drill Bit Plain Shank/Jacob Chuck End Ø4.0mm x Length 300mm for Expert Tibia Nail (Suprapatellar Insertion)



7-112-53

Stopper for Ø4.0mm Drill Bit - Expert Tibia Nail (Suprapatellar Insertion)



7-112-54

Allen Key, Hex 3mm for Expert Tibia Nail (Suprapatellar Insertion)



7-112-55

Depth Gauge measuring upto 90mm for Expert Tibia Nail (Suprapatellar Insertion)



7-112-56

Screwdriver with T-Handle, Hex 3.5mm for Expert Tibia Nail (Suprapatellar Insertion)



7-112-57

Protection Sleeve 11/8.6mm for Ø4.8mm Locking Bolt - Expert Tibia Nail (Suprapatellar Insertion)



7-112-58

Drill Sleeve 8.5/3.2mm for Ø3.2mm Drill Bit - Expert Tibia Nail (Suprapatellar Insertion)



7-112-59

Trocar Ø3.2mm for Expert Tibia Nail (Suprapatellar Insertion)



7-112-60

Drill Bit Plain Shank/Jacob Chuck End Ø3.2mm x Length 250mm for Expert Tibia Nail (Suprapatellar Insertion)



7-112-61

Stopper for Ø3.2mm Drill Bit - Expert Tibia Nail (Suprapatellar Insertion)




7-010-03

T-Handle for Flexible Reamer (AO Connection)



7-112-62

Instrument Trays for Expert Tibia Nailing Instrument Set (Suprapatellar Insertion)

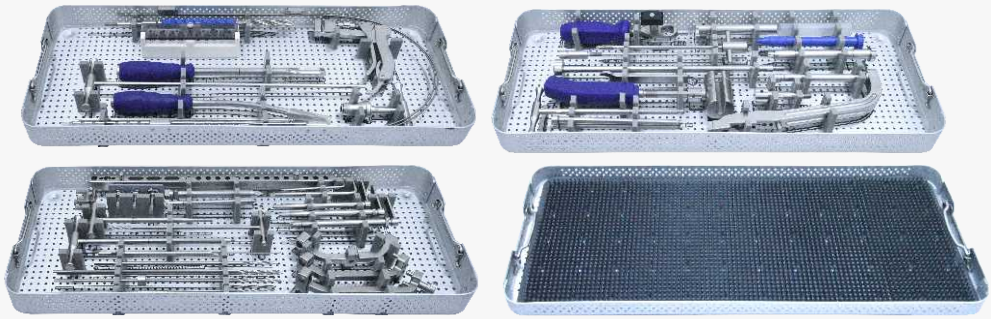


7-112-63

Container with PPSU lid for Expert Tibia Nailing Instrument Set (Suprapatellar Insertion)



7-112	Expert Tibia Nailing Instrument Set (Suprapatellar Insertion)

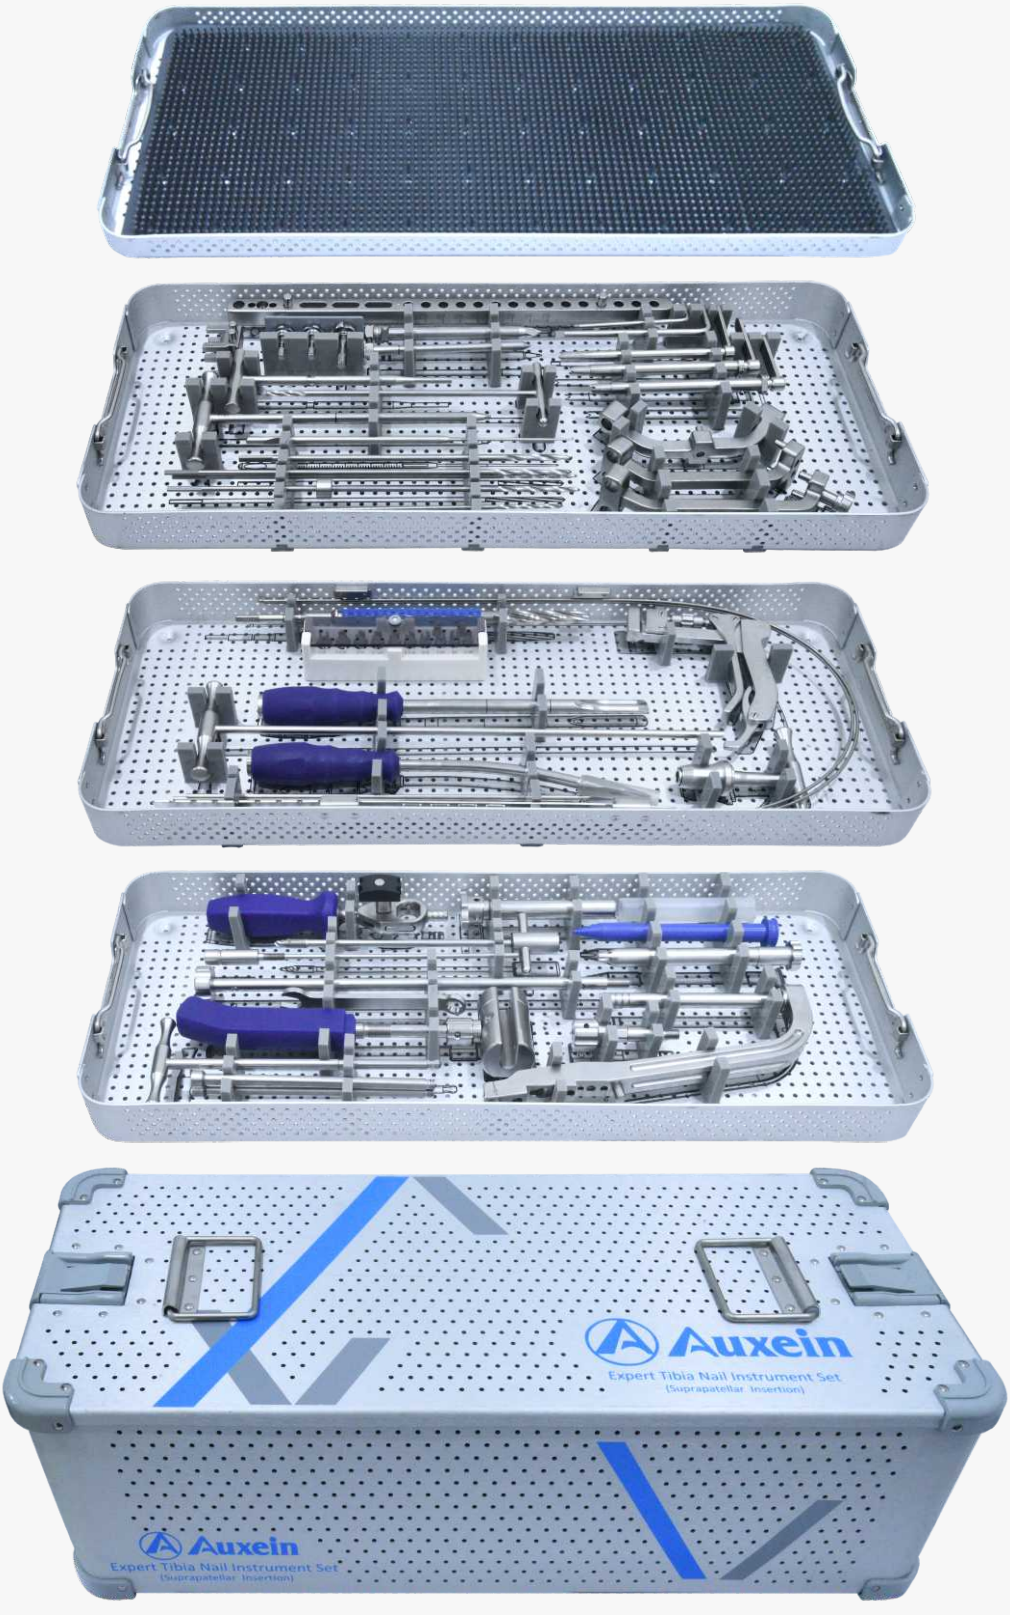

ORDER INFORMATION

7-112	Expert Tibia Nailing Instrument Set (Suprapatellar Insertion)

Code	Set Consisting Of	Unit
7-112-01	Insertion Handle for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-02	Protection Sleeve Handle for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-03	Outer Protection Sleeve for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-04	Protection Sleeve 16/14.5mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-05	Trocar Ø14.5mm, PEEK, for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-06	Centering Sleeve 14.5/3.2mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-07	Proximal Aiming Device for Ø4.4mm Locking Bolt - Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-08	Bolt for Proximal Aiming Device - Expert Tibia Nail (Suprapatellar Insertion)	2
7-112-09	Proximal Aiming Device for Ø4.8mm Locking Bolt - Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-10	Positioning Rod For Expert Tibia Nail - Suprapatellar Insertion	1
7-112-11	Stabilizing Device for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-12	Distal Aiming Arm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-13	Bolt for Distal Targeting Device, for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-14	Universal Driver for Nail Holding Bolt - Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-15	Entry Reamer for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-16	Compression Device for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-17	Extraction Screw for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-18	Connecting Shaft for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-19	Nail Holding Bolt, Long, for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-20	Combination Wrench 11mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-21	Sliding Hammer for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-22	Hammer Guide Shaft for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-23	Nut for Hammer Guide Shaft - Expert Tibia Nail - Suprapatellar Insertion	1
7-112-24	Radiographic Ruler for Expert Tibia Nail - Suprapatellar Insertion	1
520-004	Guide Wire With Threaded Tip Ø3.2mm x Thread Length 10mm x Length 300mm	3
7-112-25	Entry Cutter for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-26	Quick Coupling T Handle for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-27	Cannulated Awl for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-28	Reduction Device for Expert Tibia Nail - Suprapatellar Insertion	1
520-013	Guide wire with Ball Tip Ø2.5/3.65mm x Length 1000mm - Nitinol, for Expert Tibia Nail	1
520-058	Guide wire without Ball Tip Ø2.5mm x Length 1000mm - Nitinol, for Expert Tibia Nail	1
7-112-29	Guide Wire Holder for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-30	Flexible Reamer Shaft (AO Connection) for Expert Tibia Nail - Suprapatellar Insertion, Length 620mm	2

7-112	Expert Tibia Nailing Instrument Set (Suprapatellar Insertion)

Code	Set Consisting Of	Unit
7-010-03	T-Handle for Flexible Reamer (AO Connection)	1
7-112-31	Reamer Head, Ø7.5mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-32	Reamer Head, Ø8.0mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-33	Reamer Head, Ø8.5mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-34	Reamer Head, Ø9.0mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-35	Reamer Head, Ø9.5mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-36	Reamer Head, Ø10.0mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-37	Reamer Head, Ø10.5mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-38	Reamer Head, Ø11.0mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-39	Reamer Head, Ø11.5mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-40	Reamer Head, Ø12.0mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-41	Reamer Head, Ø12.5mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-42	Reamer Head, Ø13.0mm for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-43	Distal Aiming Device for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-44	Ø5.2mm T-Handle Drill Bit with Flat End for Expert Tibia Nail - Suprapatellar Insertion	1
7-112-45	Bolt for Distal Aiming Arm - Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-46	Allen Key, Hex 5mm for Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-47	Drill Sleeve, Ø5.2mm for Positioning Rod - Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-48	Drill Bit Plain Shank/ Jacob Chuck End Ø5.2mm x Length 250mm for Expert Tibia Nail (Suprapatellar Insertion)	2
7-112-49	Protection Drill Sleeve 10/8mm for Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-50	Trocar Ø8mm for Expert Tibia Nail (Suprapatellar Insertion)	2
7-112-51	Drill Sleeve 8/4mm for Ø4mm Drill Bit - Expert Tibia Nail (Suprapatellar Insertion)	3
7-112-52	Drill Bit Plain Shank/Jacob Chuck End Ø4.0mm x Length 300mm for Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-53	Stopper for Ø4.0mm Drill Bit - Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-54	Allen Key, Hex 3mm for Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-55	Depth Gauge measuring upto 90mm for Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-56	Screwdriver with T-Handle, Hex 3.5mm for Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-57	Protection Sleeve 11/8.6mm for Ø4.8mm Locking Bolt - Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-58	Drill Sleeve 8.5/3.2mm for Ø3.2mm Drill Bit - Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-59	Trocar Ø3.2mm for Expert Tibia Nail (Suprapatellar Insertion)	2
7-112-60	Drill Bit Plain Shank/Jacob Chuck End Ø3.2mm x Length 250mm for Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-61	Stopper for Ø3.2mm Drill Bit - Expert Tibia Nail (Suprapatellar Insertion)	1
7-112-62	Instrument Trays for Expert Tibia Nailing Instrument Set (Suprapatellar Insertion)	4
7-112-63	Container with PPSU lid for Expert Tibia Nailing Instrument Set (Suprapatellar Insertion)	1

EXPERT TIBIA NAILING (SUPRAPATELLAR INSERTION)

The content of this catalogue is intended for healthcare professionals only. All product information, illustrations, descriptions, and specifications provided here are for general informational purposes and are subject to change without notice. Auxein Medical Pvt. Ltd. reserves the right to improve or discontinue products at any time without prior notification.

This document does not constitute medical advice. Surgeons and medical practitioners must exercise their own professional judgment when using any medical devices or instruments, including those provided by Auxein.

CLINICAL USE

The implants and instruments in this catalogue are intended for use by qualified orthopedic surgeons. Improper selection, misuse, or lack of experience may result in complications.

REGULATORY COMPLIANCE

CE Approved (EUMDR-2017/745)
USFDA 510(k)
ISO 13485:2016
CDSCO
MDSAP

DISCLAIMER: Not all products in this catalogue are covered by European CE, US FDA, or other certifications. Please contact our Sales Team for product-specific certification details.

INTELLECTUAL PROPERTY

All trademarks, trade names, brand names, product names, and logos mentioned in this catalogue are the property of Auxein Medical Pvt. Ltd. Unauthorized use or reproduction is strictly prohibited.

V1-2026

SCAN TO KNOW MORE

INDIA
AUXEIN MEDICAL PVT.LTD.

PLOT NO. 168-169-170, PHASE-4,
KUNDLI INDUSTRIAL AREA,
HSIIDC, SECTOR-57,
SONEPAT-131028, HARYANA
TEL: +91 99106 43638
FAX: +91 86077 70197
EMAIL: INFO@AUXEIN.COM

MÉXICO
AUXEIN MÉXICO, S.A DE C.V

TEPIC 39 INT 801, COLONIA
ROMA SUR,
ALCADÍA CUAUHTÉMOC, CDMX
MÉXICO, C.P 06760
TEL: +521 55 7261 0318
EMAIL: INFO@AUXEIN.MX

USA
AUXEIN INC.

1500 NW 89TH COURT,
SUITE 107-108
DORAL,FLORIDA 33172
TEL. +1 305 395 6062
E FAX:+1 305 395 62 62
EMAIL: USOFFICE@AUXEIN.COM

DUBAI UAE
AUXEIN MEDICAL

TRADING FZCO OUD METHA
OFFICES BUILDING B BLOCK,
1ST FLOOR, OFFICE NO.26,
NEAR HEALTHCARE CITY,
PO BOX-25572
TEL. +971 438 71333
EMAIL: INFO@AUXEIN.COM

WWW.AUXEIN.COM